

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
 Data File : BG045585.D
 Acq On : 3 Jun 2020 17:39
 Operator : CG/JU
 Sample : L2839-25
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NM-EB-09

Quant Time: Jun 03 18:40:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	58882	20.00	ng	0.00
21) Naphthalene-d8	10.76	136	232299	20.00	ng	0.00
39) Acenaphthene-d10	14.60	164	166169	20.00	ng	0.00
64) Phenanthrene-d10	17.34	188	395768	20.00	ng	0.00
76) Chrysene-d12	21.60	240	409179	20.00	ng	0.00
87) Perylene-d12	24.76	264	427614	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	156253	51.86	ng	0.00
7) Phenol-d6	7.15	99	132941	31.00	ng	0.00
23) Nitrobenzene-d5	9.11	82	392289	92.09	ng	0.00
42) 2,4,6-Tribromophenol	16.09	330	322753	151.88	ng	0.00
45) 2-Fluorobiphenyl	13.22	172	923688	94.29	ng	0.00
79) Terphenyl-d14	19.96	244	1824828	104.01	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.05	163	131108	11.502	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
Data File : BG045585.D
Acq On : 3 Jun 2020 17:39
Operator : CG/JU
Sample : L2839-25
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NM-EB-09

Quant Time: Jun 03 18:40:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

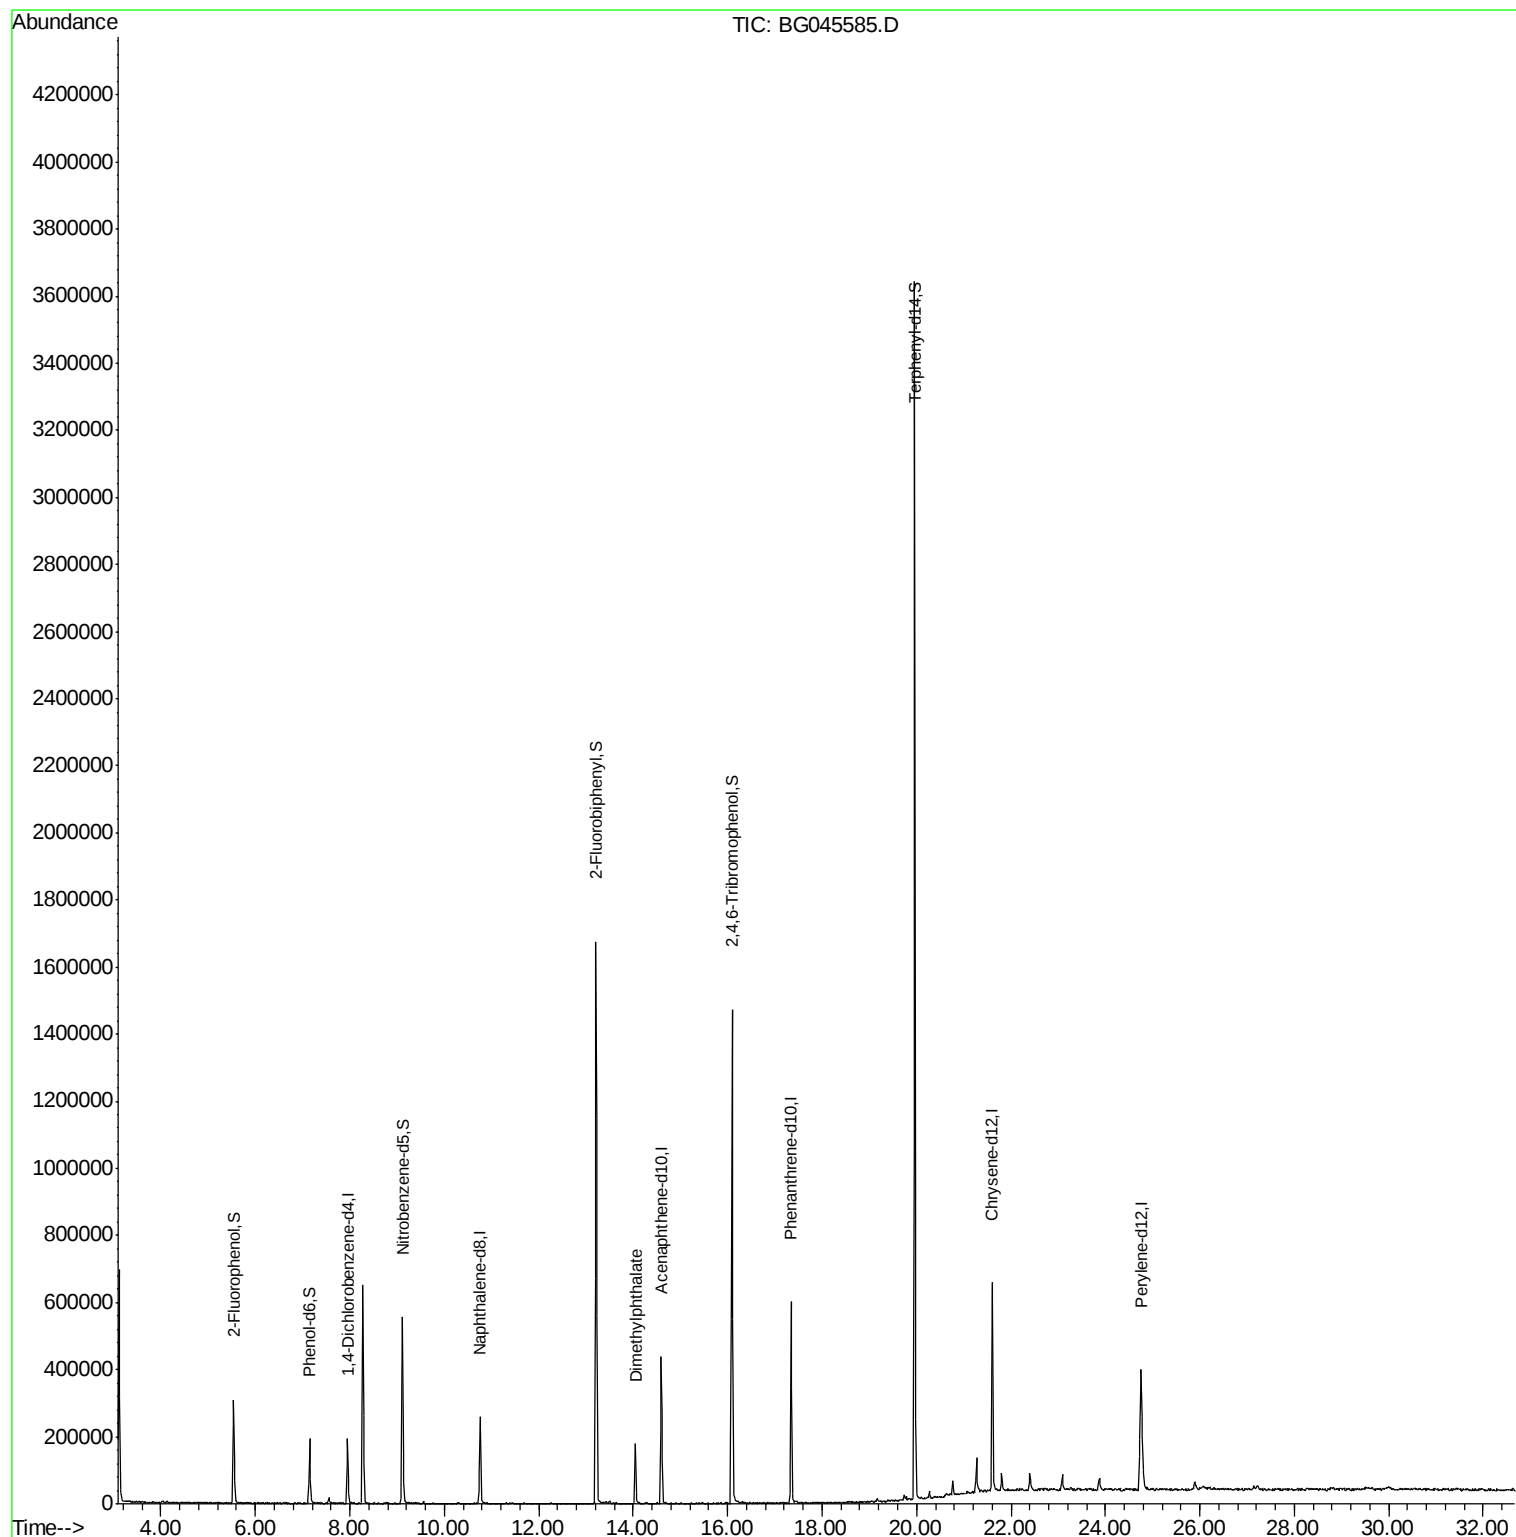

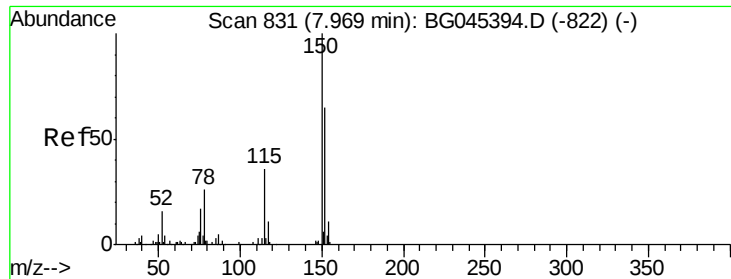


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.95 min Scan# 828
Delta R.T. 0.00 min
Lab File: BG045585.D
Acq: 3 Jun 2020 17:39

Instrument :
BNA_G
ClientSampleId :
NM-EB-09

Tot Ion:152 Resp: 58882
Ion Ratio Lower Upper
152 100
150 156.7 122.4 183.6
115 60.6 44.2 66.4

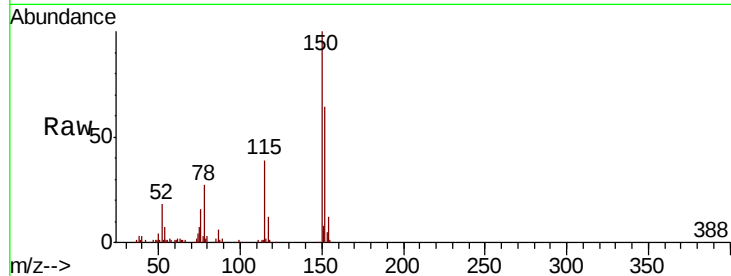


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

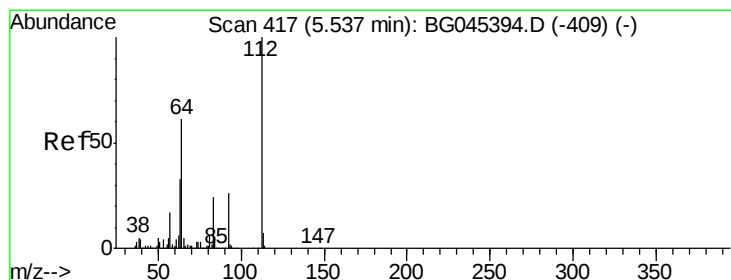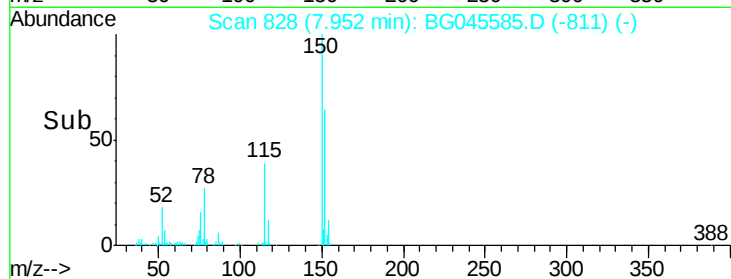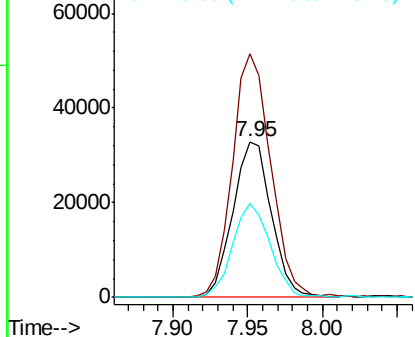



#5


2-Fluorophenol
Concen: 51.860 ng
RT: 5.54 min Scan# 417
Delta R.T. 0.00 min
Lab File: BG045585.D
Acq: 3 Jun 2020 17:39

Tgt Ion:112 Resp: 156253
Ion Ratio Lower Upper
112 100
64 58.2 48.6 72.8
63 31.5 26.5 39.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

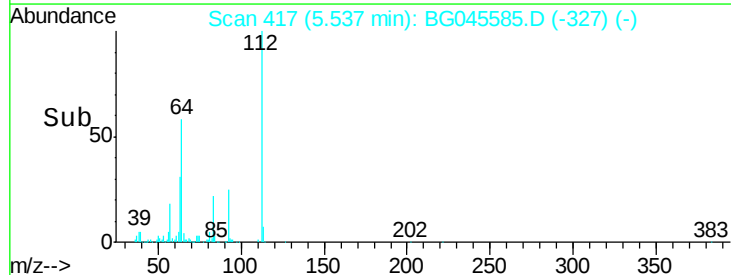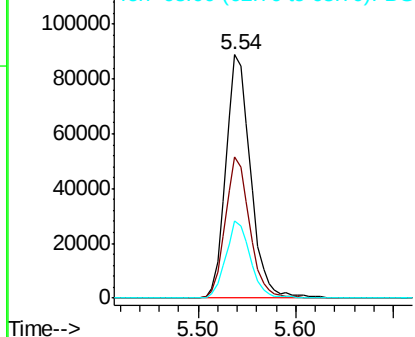



#7

Phenol-d6

Concen: 31.001 ng

RT: 7.15 min Scan# 691

Delta R.T. 0.00 min

Lab File: BG045585.D

Acq: 3 Jun 2020 17:39

Instrument :

BNA_G

ClientSampleId :

NM-EB-09


Tot Ion: 99 Resp: 132941

Ion Ratio Lower Upper




99 100

42 14.9 11.3 16.9

71 40.0 30.8 46.2

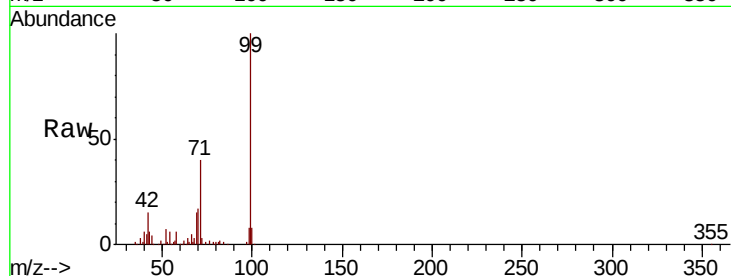

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

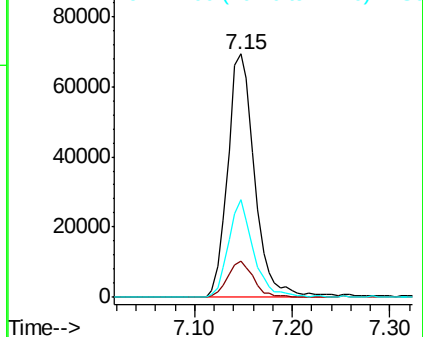

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.76 min Scan# 1306

Delta R.T. 0.00 min

Lab File: BG045585.D

Acq: 3 Jun 2020 17:39

Tgt Ion: 136 Resp: 232299


Ion Ratio Lower Upper

136 100



137 11.2 9.4 14.2


54 5.7 5.8 8.6#

68 4.8 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




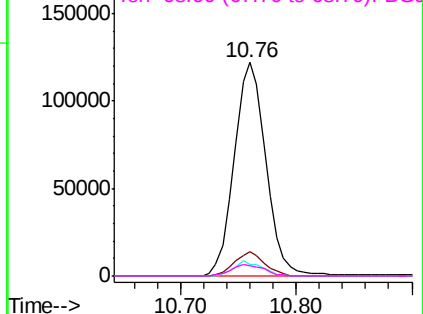




#23
Nitrobenzene-d5
Concen: 92.089 ng
RT: 9.11 min Scan# 1026
Delta R.T. 0.00 min
Lab File: BG045585.D
Acq: 3 Jun 2020 17:39




Instrument :
BNA_G
ClientSampleId :
NM-EB-09


Tot Ion	82	Resp	392289
Ion Ratio	Lower	Upper	
82	100		
128	40.3	30.9	46.3
54	40.5	30.3	45.5

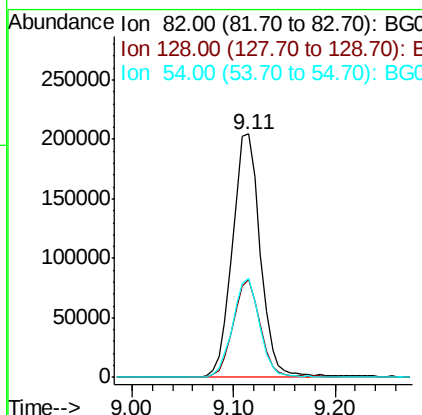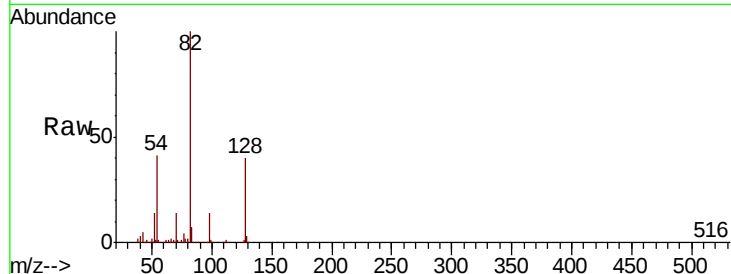

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.60 min Scan# 1959
Delta R.T. 0.00 min
Lab File: BG045585.D
Acq: 3 Jun 2020 17:39

Tgt Ion	164	Resp	166169
Ion Ratio	Lower	Upper	
164	100		
162	95.0	76.9	115.3
160	42.0	33.8	50.8

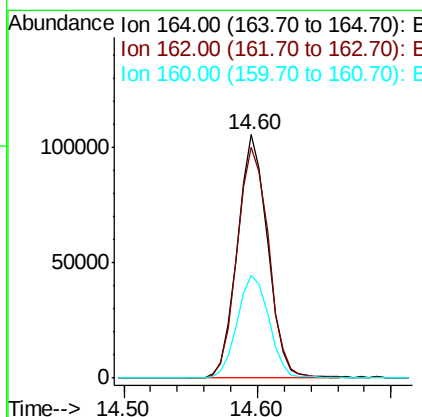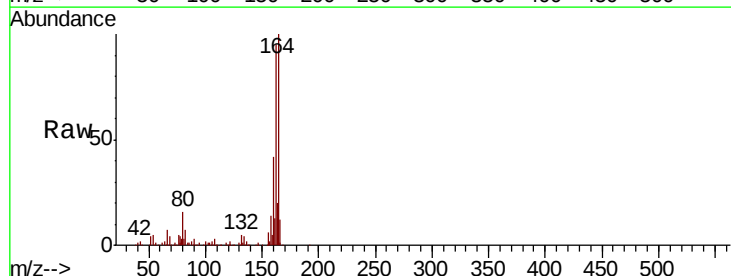







#42
 2,4,6-Tribromophenol
 Concen: 151.876 ng
 RT: 16.09 min Scan# 2214
 Delta R.T. 0.00 min
 Lab File: BG045585.D
 Acq: 3 Jun 2020 17:39

Instrument :
 BNA_G
 ClientSampleId :
 NM-EB-09

Tot Ion:330 Resp: 322753
 Ion Ratio Lower Upper
 330 100
 332 98.2 78.2 117.4
 141 34.8 28.2 42.4

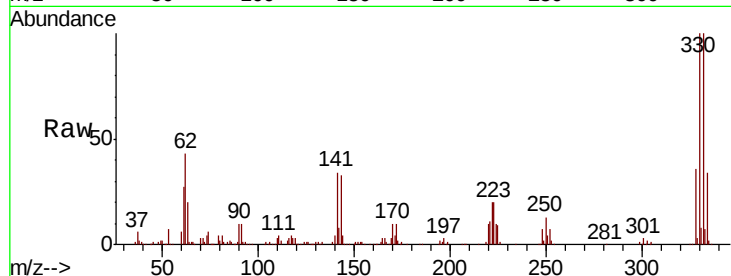


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


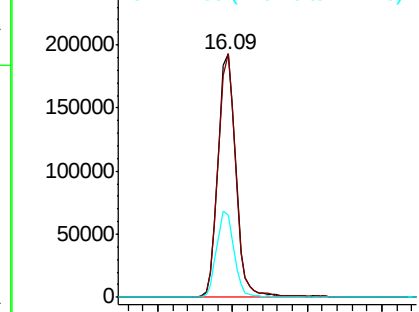


#45
 2-Fluorobiphenyl
 Concen: 94.288 ng
 RT: 13.22 min Scan# 1724
 Delta R.T. 0.00 min
 Lab File: BG045585.D
 Acq: 3 Jun 2020 17:39

Tgt Ion:172 Resp: 923688
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.5 44.3
 170 23.2 18.5 27.7



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

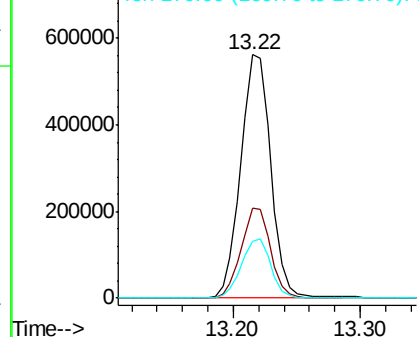



#50

Dimethylphthalate

Concen: 11.502 ng

RT: 14.05 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BG045585.D

Acq: 3 Jun 2020 17:39

Instrument :

BNA_G

ClientSampleId :

NM-EB-09


Tot Ion:163 Resp: 131108

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8




164 9.8 8.3 12.5

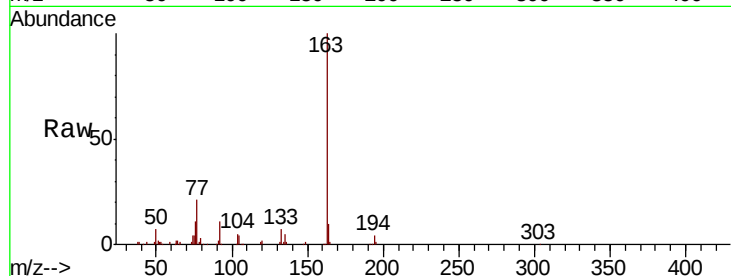

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

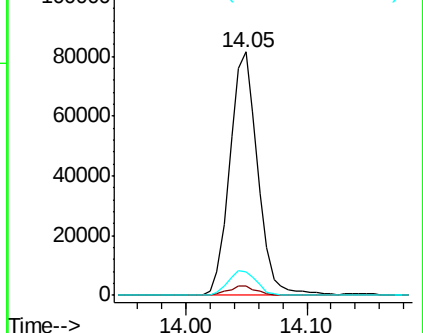

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.34 min Scan# 2427

Delta R.T. 0.00 min

Lab File: BG045585.D

Acq: 3 Jun 2020 17:39


Tgt Ion:188 Resp: 395768

Ion Ratio Lower Upper

188 100

94 7.5 5.5 8.3



80 8.8 6.6 10.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

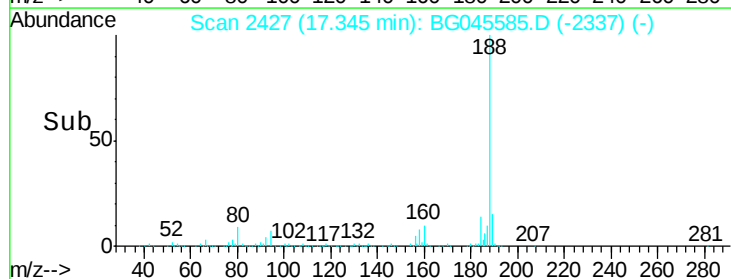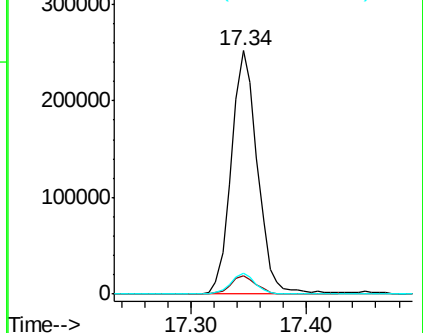

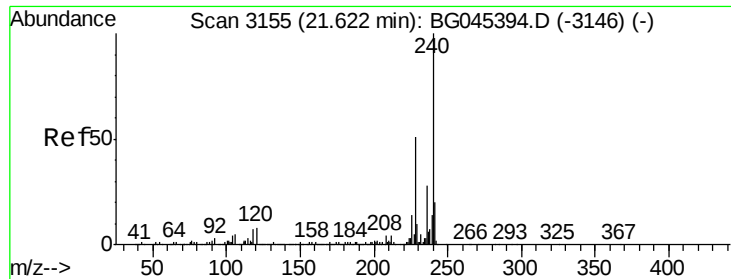

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.60 min Scan# 3152

Delta R.T. 0.00 min

Lab File: BG045585.D

Acq: 3 Jun 2020 17:39

Instrument :

BNA_G

ClientSampleId :

NM-EB-09


Tot Ion:240 Resp: 409179

Ion Ratio Lower Upper

240 100

120 7.3 6.1 9.1




236 26.9 22.3 33.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

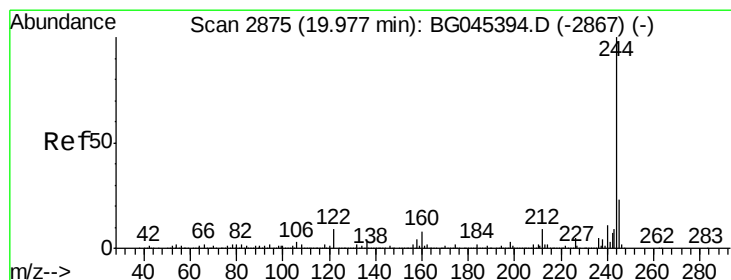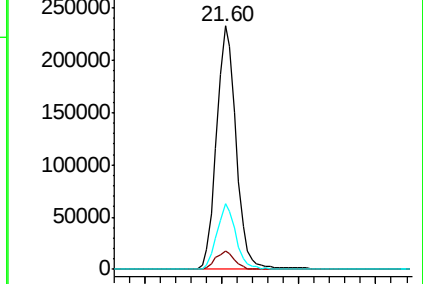

#79

Terphenyl-d14

Concen: 104.014 ng

RT: 19.96 min Scan# 2873

Delta R.T. 0.01 min

Lab File: BG045585.D

Acq: 3 Jun 2020 17:39


Tgt Ion:244 Resp: 1824828

Ion Ratio Lower Upper

244 100

212 9.3 7.4 11.0



122 8.7 6.8 10.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

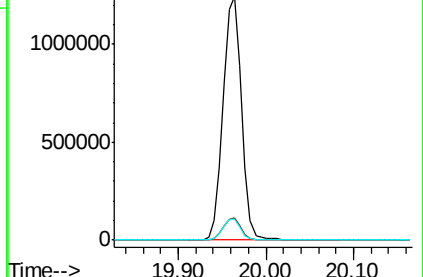


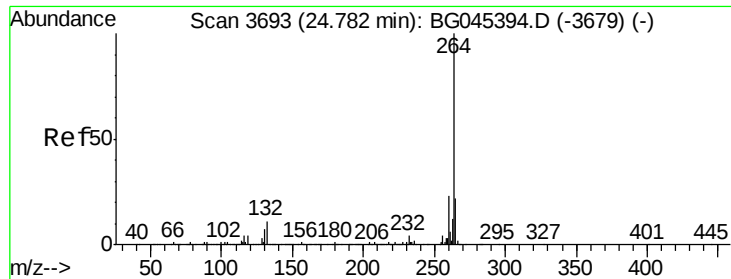

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.76 min Scan# 3689
 Delta R.T. 0.01 min
 Lab File: BG045585.D
 Acq: 3 Jun 2020 17:39

Instrument :
 BNA_G
 ClientSampleId :
 NM-EB-09

Tot Ion:	264	Resp:	427614
Ion	Ratio	Lower	Upper
264	100		
260	21.6	18.2	27.4
265	21.8	17.6	26.4



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

