

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
 Data File : BG045585.D
 Acq On : 3 Jun 2020 17:39
 Operator : CG/JU
 Sample : L2839-25
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NM-EB-09

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.537	411	417	427	rBV	308078	541034	10.53%	2.851%
2	7.147	684	691	705	rBV	192981	362065	7.04%	1.908%
3	7.952	822	828	836	rBV	194357	349068	6.79%	1.839%
4	8.275	876	883	893	rBV	651578	1177169	22.90%	6.203%
5	9.115	1017	1026	1040	rBV	555504	1051522	20.46%	5.541%
6	10.760	1299	1306	1319	rBV	258306	483000	9.40%	2.545%
7	13.215	1717	1724	1736	rBV	1673753	2694582	52.42%	14.198%
8	14.049	1859	1866	1877	rBV	179525	292563	5.69%	1.542%
9	14.596	1953	1959	1967	rBV	438869	715331	13.92%	3.769%
10	16.094	2207	2214	2226	rBV	1472479	2452297	47.71%	12.922%
11	17.345	2421	2427	2437	rBV	601801	946061	18.40%	4.985%
12	19.965	2866	2873	2884	rBV	3629487	5140257	100.00%	27.085%
13	20.770	3004	3010	3013	rBV2	44407	57819	1.12%	0.305%
14	21.269	3090	3095	3108	rVB2	100319	184295	3.59%	0.971%
15	21.604	3146	3152	3162	rBV2	617935	1067079	20.76%	5.623%
16	21.803	3182	3186	3192	rBV2	50210	77429	1.51%	0.408%
17	22.403	3283	3288	3295	rBV4	47775	80541	1.57%	0.424%
18	23.084	3398	3404	3411	rBV3	45980	94737	1.84%	0.499%
19	23.871	3533	3538	3547	rVB4	33865	79679	1.55%	0.420%
20	24.752	3679	3688	3704	rBV2	357126	1131526	22.01%	5.962%


Sum of corrected areas: 18978054

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
Data File : BG045585.D
Acq On : 3 Jun 2020 17:39
Operator : CG/JU
Sample : L2839-25
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NM-EB-09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

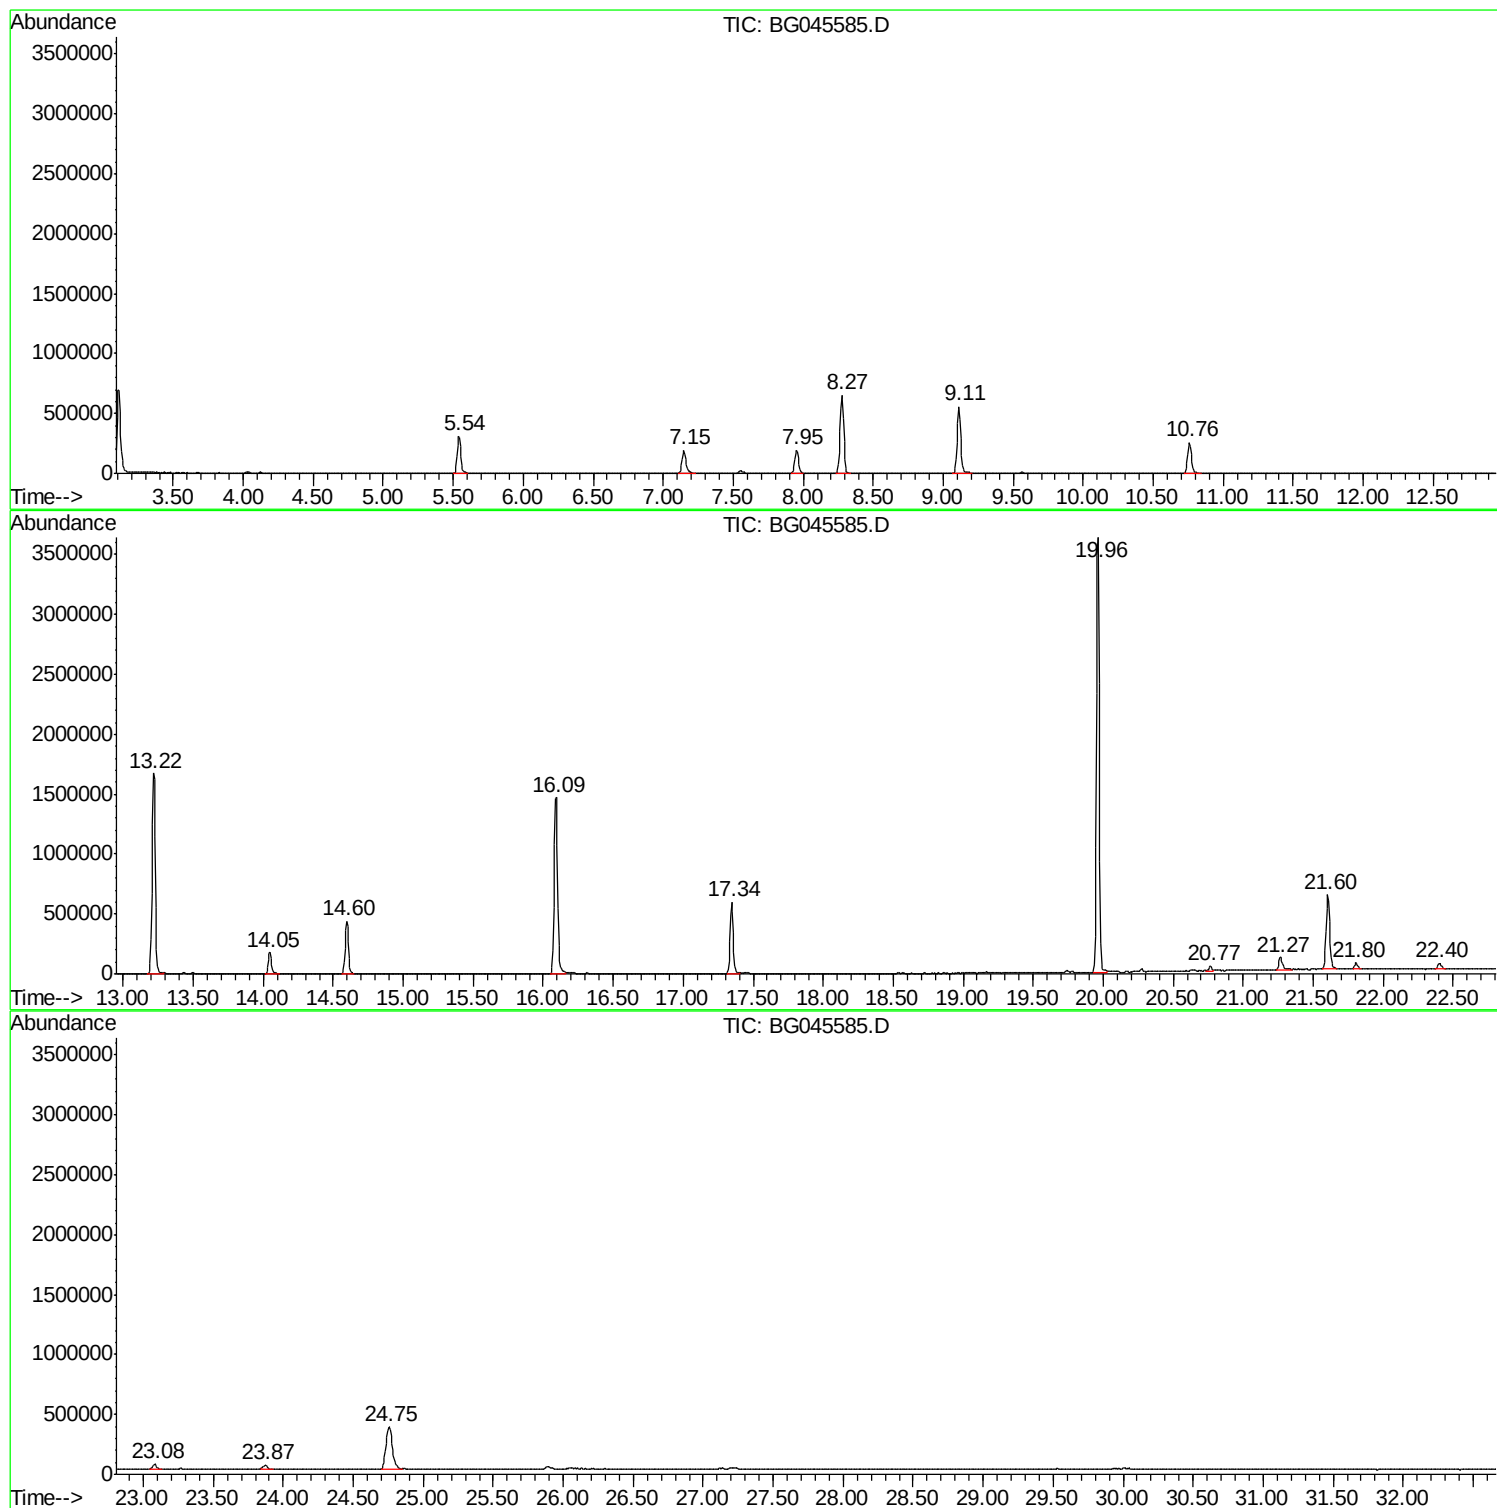

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060320\
Data File : BG045585.D
Acq On : 3 Jun 2020 17:39
Operator : CG/JU
Sample : L2839-25
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
NM-EB-09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Oxalic acid, isobutyl penta... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.		
21.27	3.45 ng	184295	Chrysene-d12	21.60		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Oxalic acid, isobutyl pentadecyl...	356	C21H40O4	1000309-38-0	91	
2	Oxalic acid, isobutyl tetradecyl...	342	C20H38O4	1000309-37-9	90	
3	Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	86	
4	Oxalic acid, hexadecyl propyl ester	356	C21H40O4	1000309-26-9	74	
5	2-methyltetracosane	352	C25H52	1000376-72-6	52	

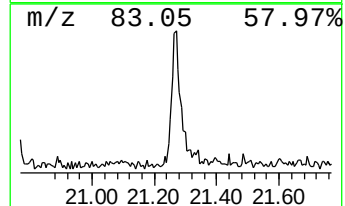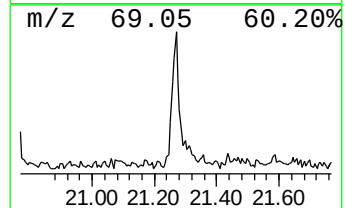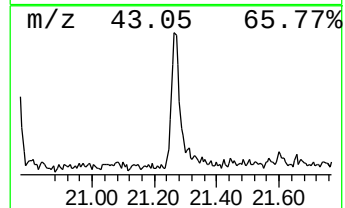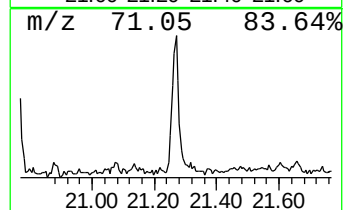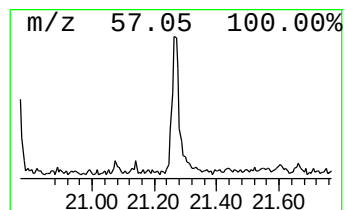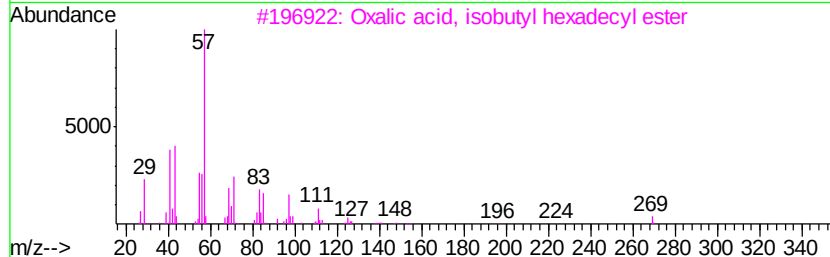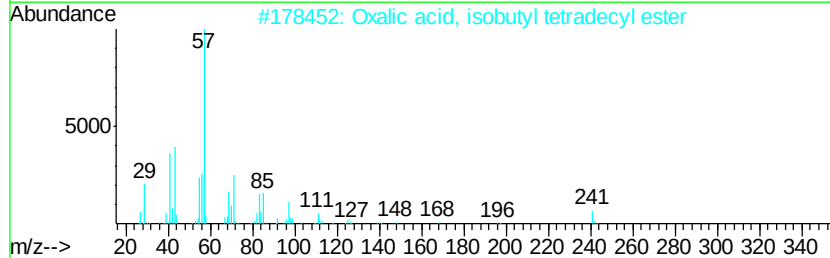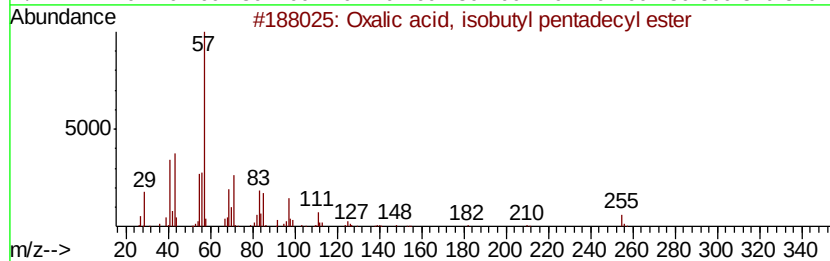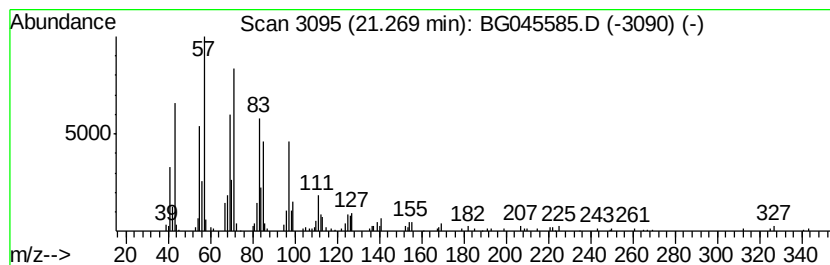

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060320\
Data File : BG045585.D
Acq On : 3 Jun 2020 17:39
Operator : CG/JU
Sample : L2839-25
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NM-EB-09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Oxalic acid, isob...	21.27	3.5	ng	184295	5	21.60	1067080	20.0