

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
 Data File : BG053808.D
 Acq On : 3 Jun 2022 11:42
 Operator : CG/JU
 Sample : N2987-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P033-SS001-2430-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.656	378	386	397	rBV	317213	549900	34.45%	8.177%
2	7.237	647	655	664	rBV	322736	570078	35.71%	8.477%
3	8.089	794	800	807	rVB	77138	137145	8.59%	2.039%
4	9.246	989	997	1005	rBV	191475	355290	22.26%	5.283%
5	10.897	1269	1278	1287	rBV	102164	193074	12.10%	2.871%
6	13.341	1686	1694	1701	rVB	506344	825021	51.69%	12.269%
7	14.710	1920	1927	1935	rVB	174533	277462	17.38%	4.126%
8	16.191	2171	2179	2189	rBV	456062	729178	45.68%	10.843%
9	17.454	2387	2394	2401	rBV	250404	381823	23.92%	5.678%
10	20.063	2832	2838	2844	rBV	1210094	1596190	100.00%	23.736%
11	21.379	3056	3062	3075	rBV	95246	164440	10.30%	2.445%
12	21.732	3114	3122	3130	rBV2	282318	475716	29.80%	7.074%
13	22.572	3260	3265	3274	rVB6	11208	23417	1.47%	0.348%
14	24.993	3668	3677	3689	rVB2	153639	445975	27.94%	6.632%




Sum of corrected areas: 6724709

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053808.D
Acq On : 3 Jun 2022 11:42
Operator : CG/JU
Sample : N2987-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P033-SS001-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

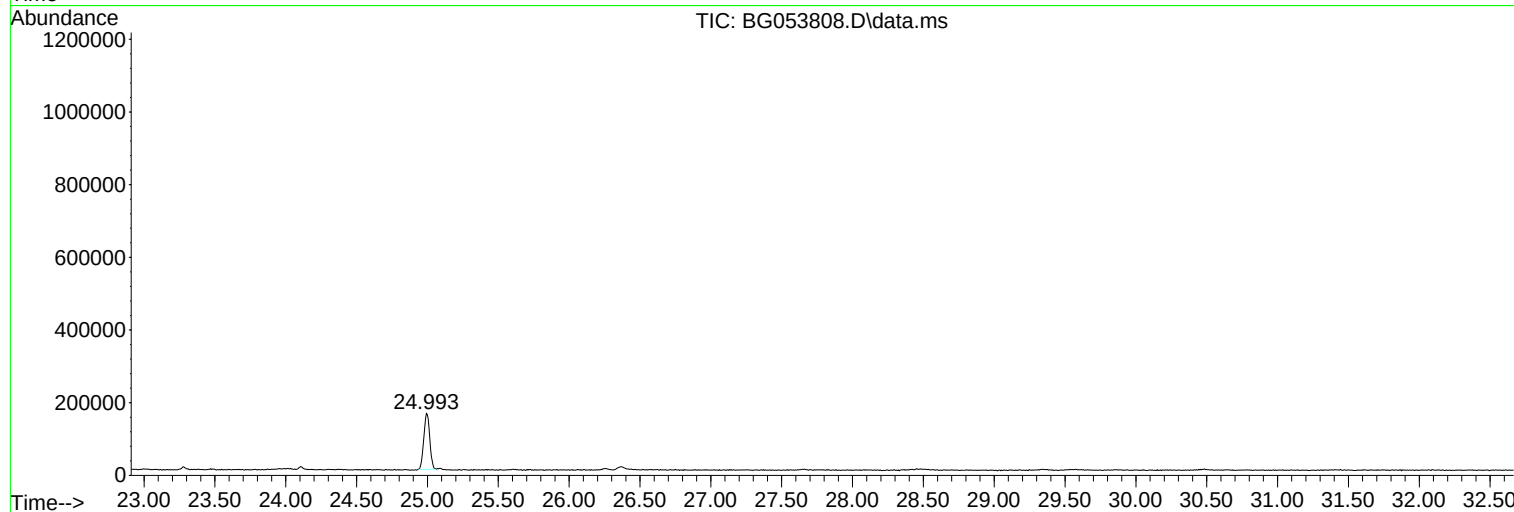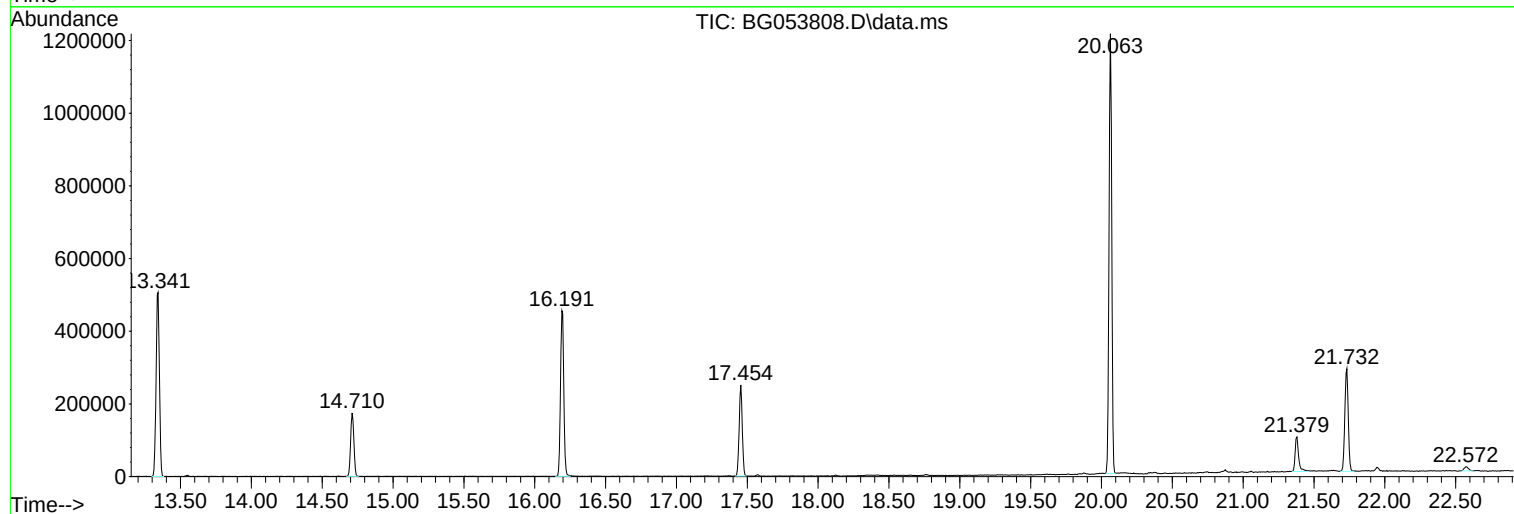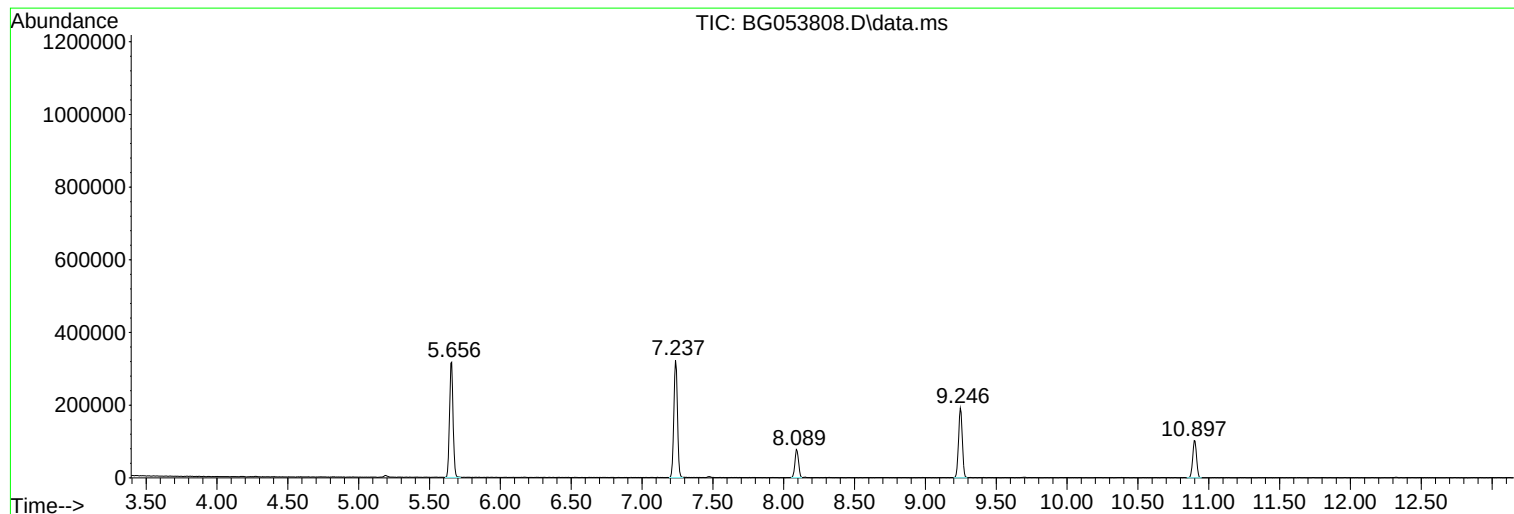

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053808.D
Acq On : 3 Jun 2022 11:42
Operator : CG/JU
Sample : N2987-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P033-SS001-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.379	6.91 ng	164440	Chrysene-d12	21.732

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
3			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
4			1-Hexacosene	364	C26H52	018835-33-1	94
5			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91

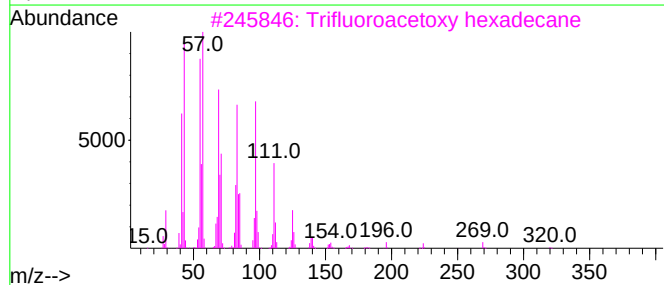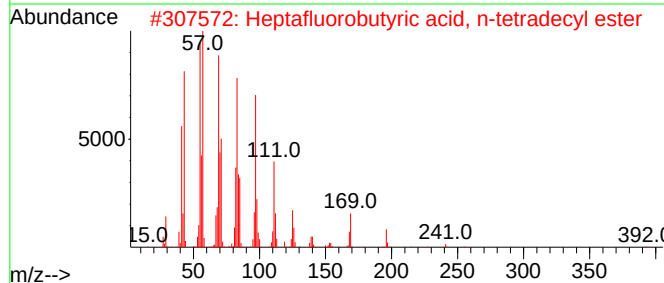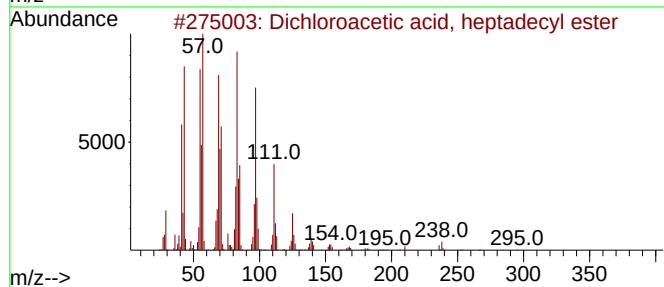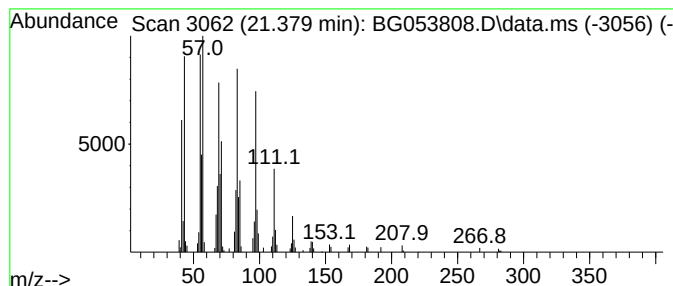

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053808.D
Acq On : 3 Jun 2022 11:42
Operator : CG/JU
Sample : N2987-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P033-SS001-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	21.379	6.9	ng	164440	5	21.732	475716	20.0