

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
 Data File : BG053812.D
 Acq On : 3 Jun 2022 14:19
 Operator : CG/JU
 Sample : N2984-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P014-SS002-2430-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.658	378	386	397	rBV	454168	772400	38.63%	8.929%
2	7.244	646	656	668	rBV	451554	821094	41.06%	9.492%
3	8.090	793	800	807	rBV	88558	158184	7.91%	1.829%
4	9.248	989	997	1007	rBV	277815	512826	25.65%	5.928%
5	10.899	1271	1278	1287	rVB	124262	228919	11.45%	2.646%
6	13.343	1685	1694	1701	rBV	765068	1272679	63.64%	14.712%
7	14.712	1920	1927	1935	rBV	206419	329781	16.49%	3.812%
8	16.193	2172	2179	2188	rBV	620396	983304	49.17%	11.367%
9	17.456	2386	2394	2402	rBV	266322	417045	20.86%	4.821%
10	18.343	2541	2545	2554	rBV2	16974	27709	1.39%	0.320%
11	20.065	2832	2838	2844	rBV	1479978	1999655	100.00%	23.116%
12	20.876	2970	2976	2979	rBV4	14613	22221	1.11%	0.257%
13	21.381	3057	3062	3069	rVB2	59392	95405	4.77%	1.103%
14	21.733	3115	3122	3129	rVB	288814	481202	24.06%	5.563%
15	21.945	3154	3158	3163	rVB4	12424	20823	1.04%	0.241%
16	22.574	3261	3265	3269	rBV5	12604	21453	1.07%	0.248%
17	24.113	3521	3527	3532	rBV4	11101	25928	1.30%	0.300%
18	25.000	3668	3678	3689	rBV2	160678	459757	22.99%	5.315%




Sum of corrected areas: 8650385

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053812.D
Acq On : 3 Jun 2022 14:19
Operator : CG/JU
Sample : N2984-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P014-SS002-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

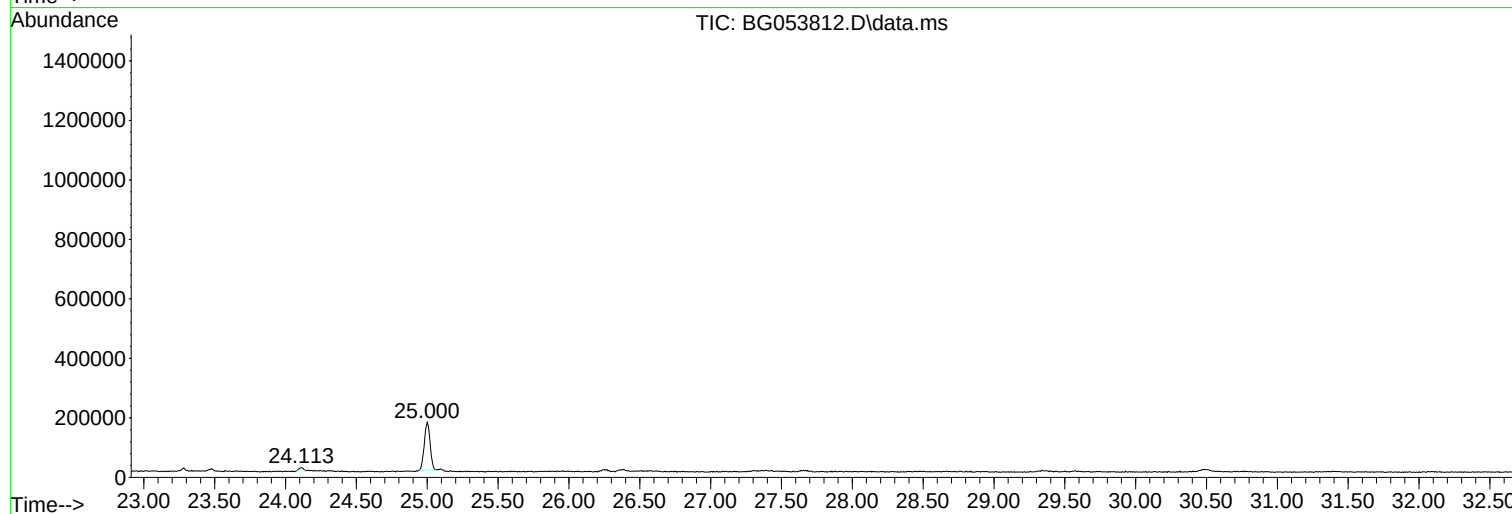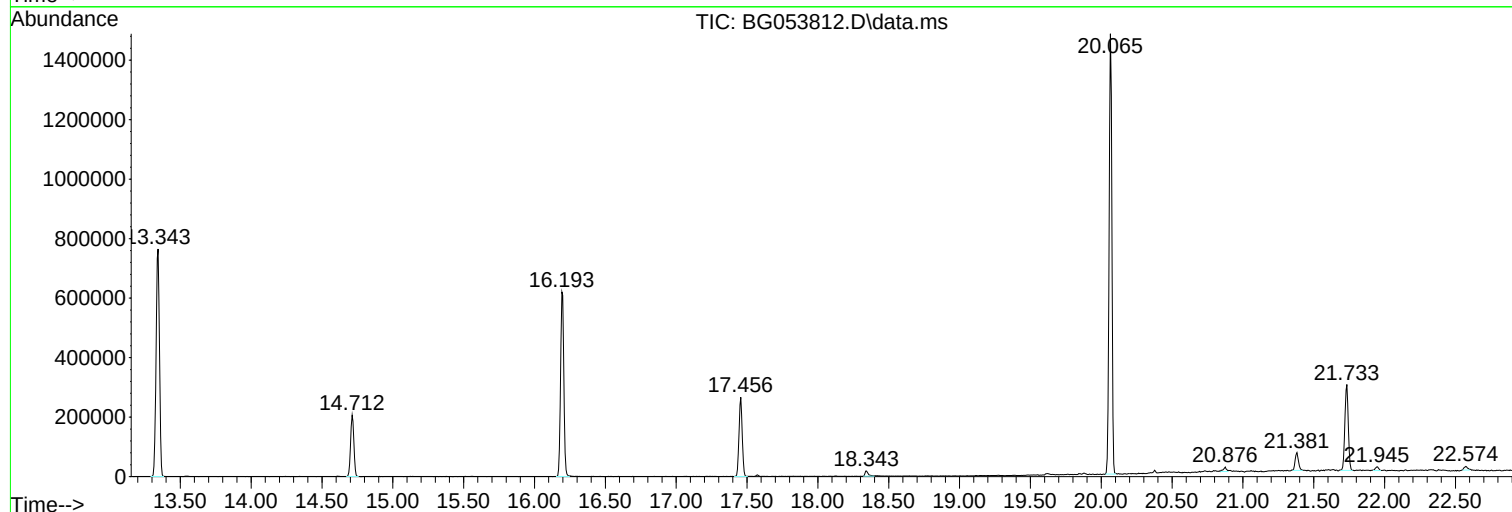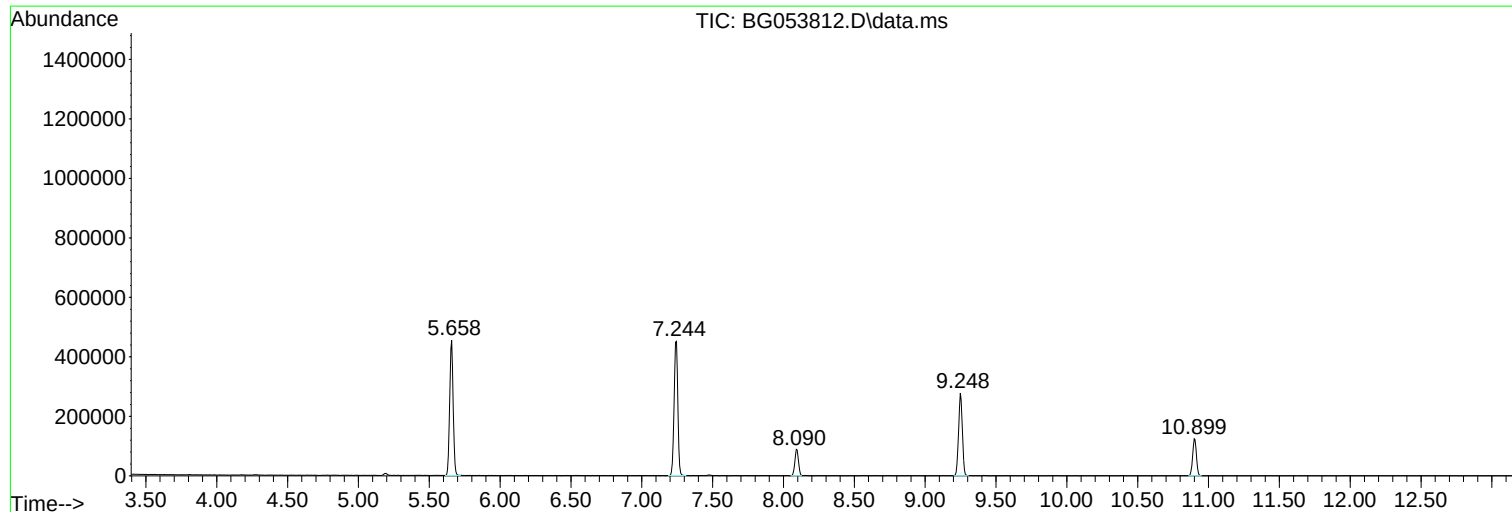

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053812.D
Acq On : 3 Jun 2022 14:19
Operator : CG/JU
Sample : N2984-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P014-SS002-2430-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.381	3.97 ng	95405	Chrysene-d12	21.733

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2			Cyclotridecane	182	C13H26	000295-02-3	94
3			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91
5			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91

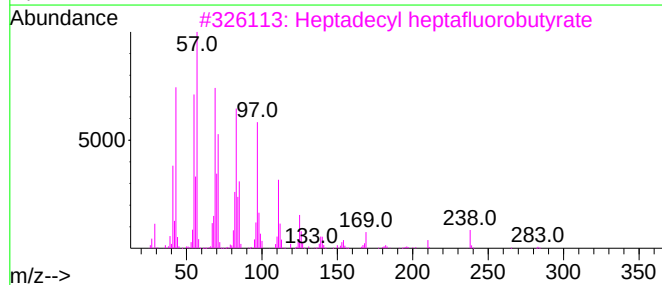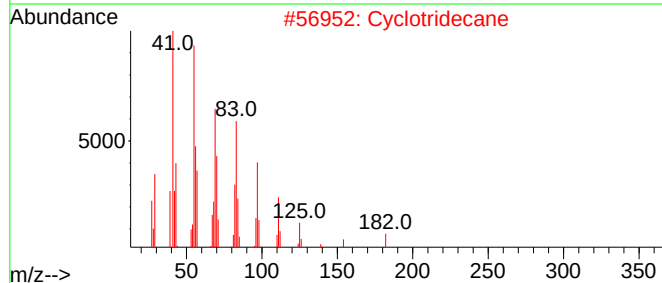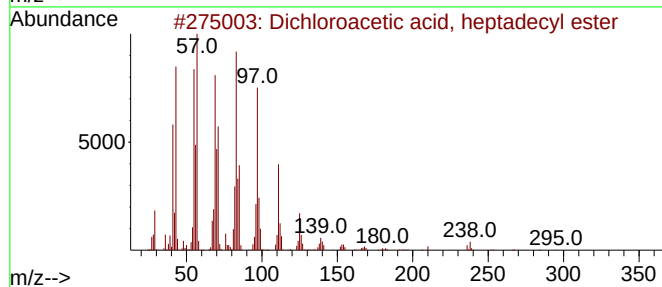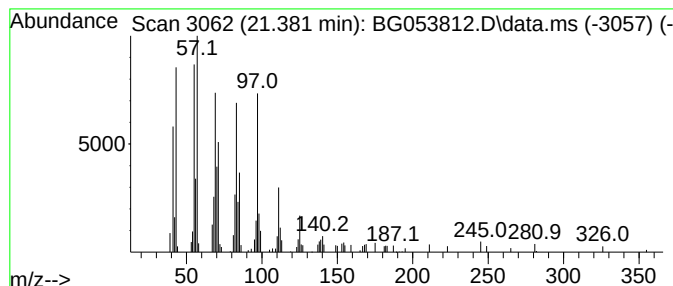

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053812.D
Acq On : 3 Jun 2022 14:19
Operator : CG/JU
Sample : N2984-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P014-SS002-2430-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	21.381	4.0	ng	95405	5	21.733	481202	20.0