
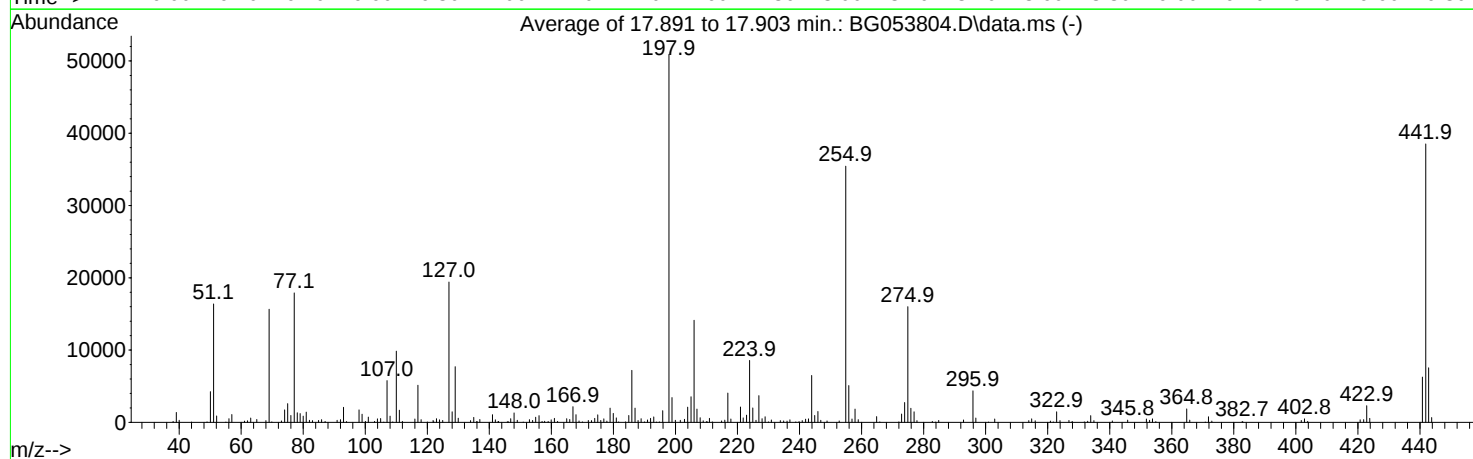


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
 Data File : BG053804.D
 Acq On : 3 Jun 2022 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

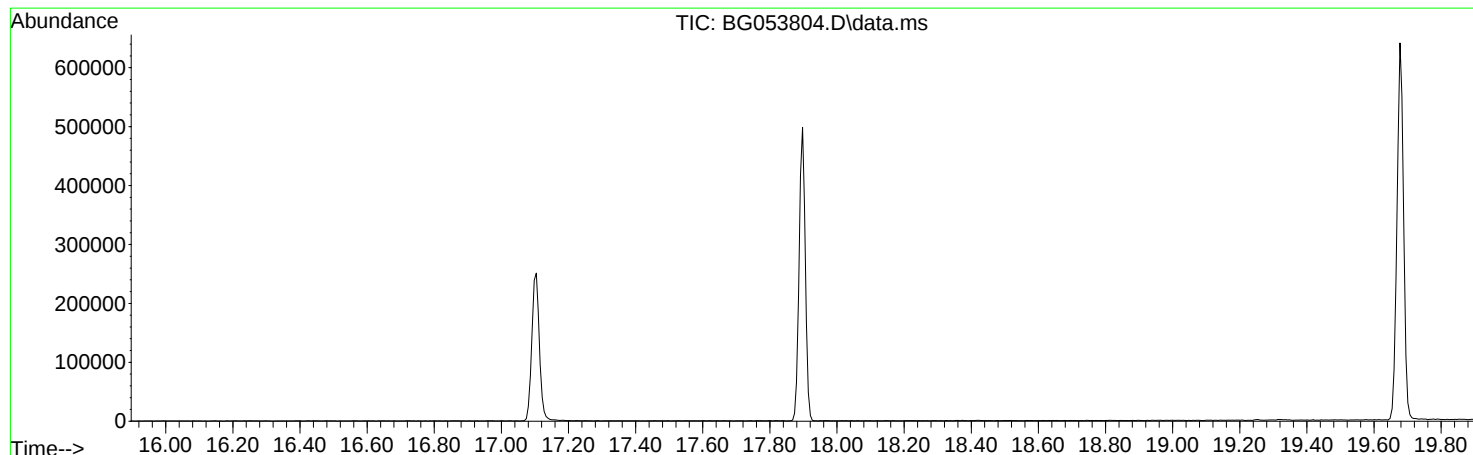

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	16388	PASS
68	69	0.00	2	1.5	237	PASS
69	198	0.00	100	30.8	15658	PASS
70	69	0.00	2	0.4	64	PASS
127	198	10	80	38.2	19418	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50896	PASS
199	198	5	9	6.8	3436	PASS
275	198	10	60	31.4	15999	PASS
365	198	1	100	3.6	1852	PASS
441	198	0.01	100	12.3	6271	PASS
442	442	50	100	100.0	38525	PASS
443	442	15	24	19.6	7551	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/3/2022	BNA_G	<u>BG053804.D</u>
Compound Name	Response	Retention Time
DDT	173972	20.92
DDD	627	20.47
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
627	174599	0.36

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053804.D
Acq On : 3 Jun 2022 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 03 14:13:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

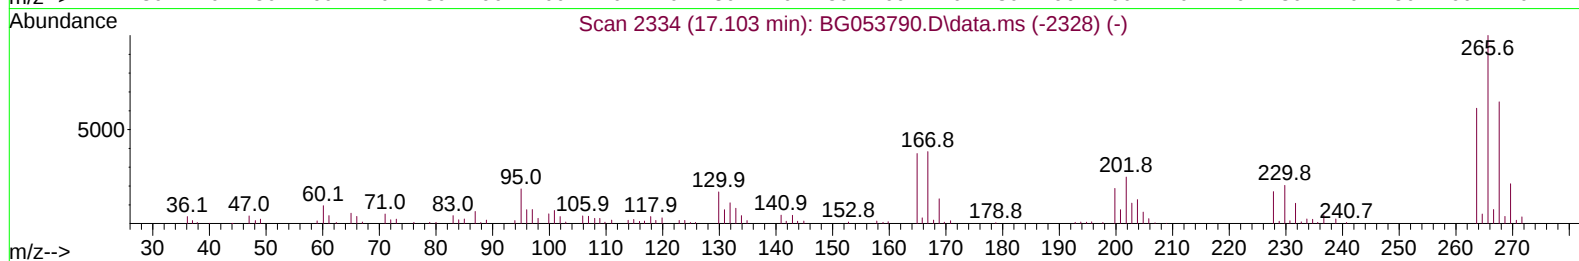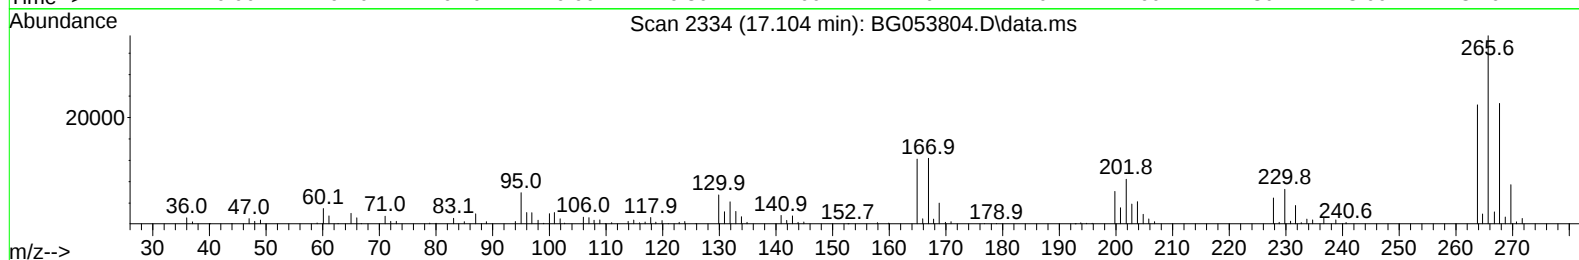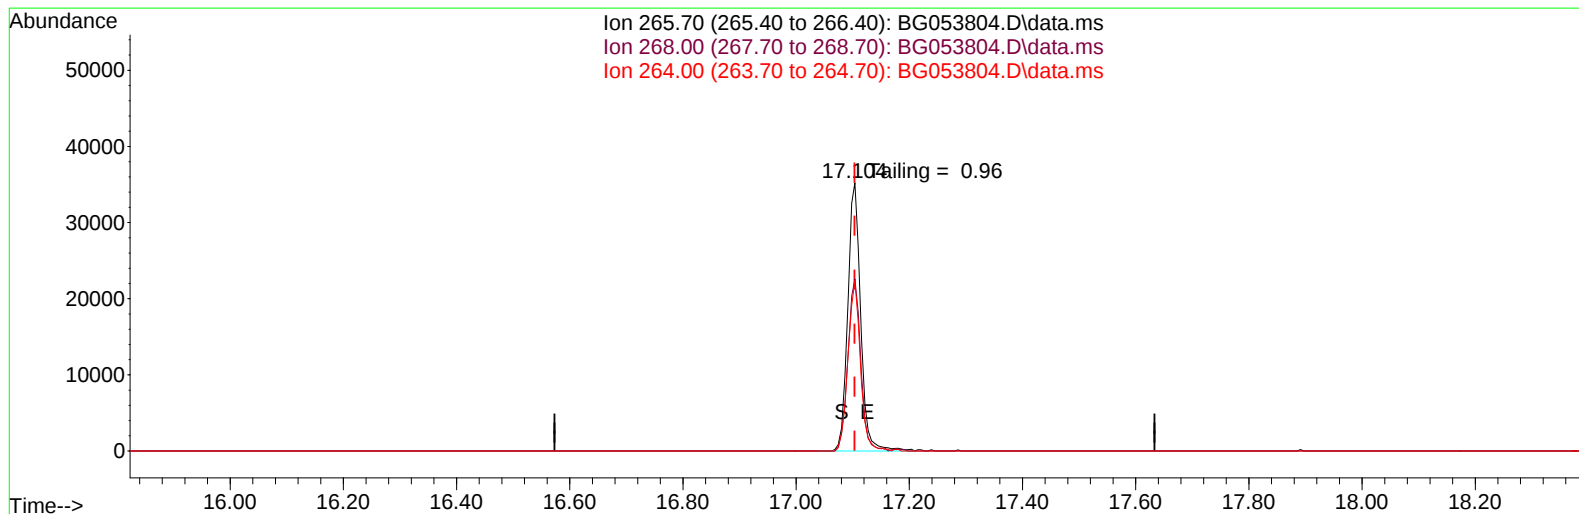

TIC: BG053804.D\data.ms

(70) Pentachlorophenol (C)

17.104min (+ 0.001) 20467.74 ng




response 55851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.18
264.00	66.20	69.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060322\
Data File : BG053804.D
Acq On : 3 Jun 2022 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 03 14:13:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

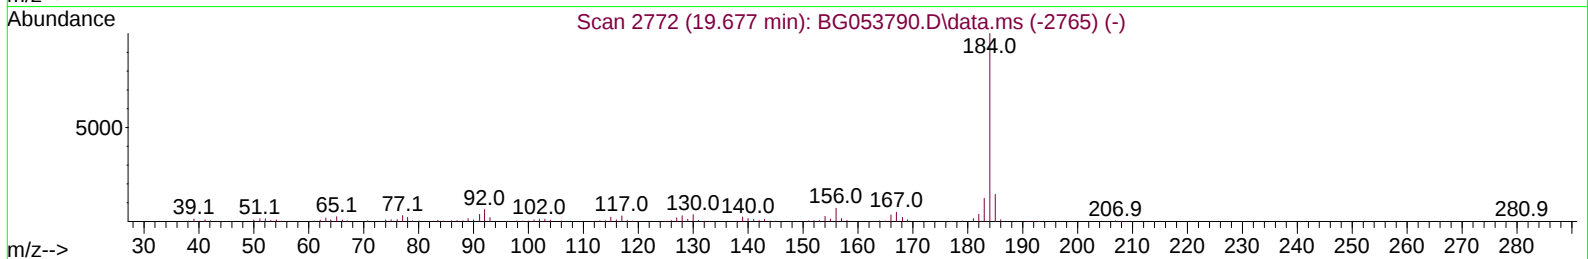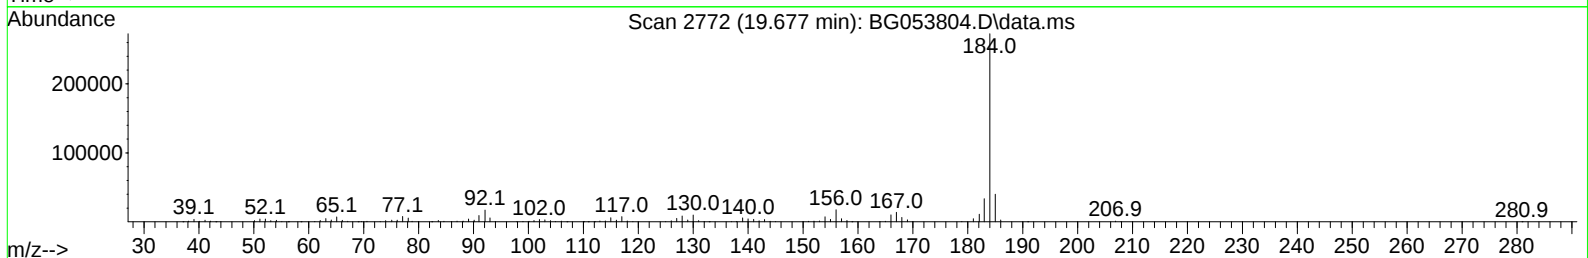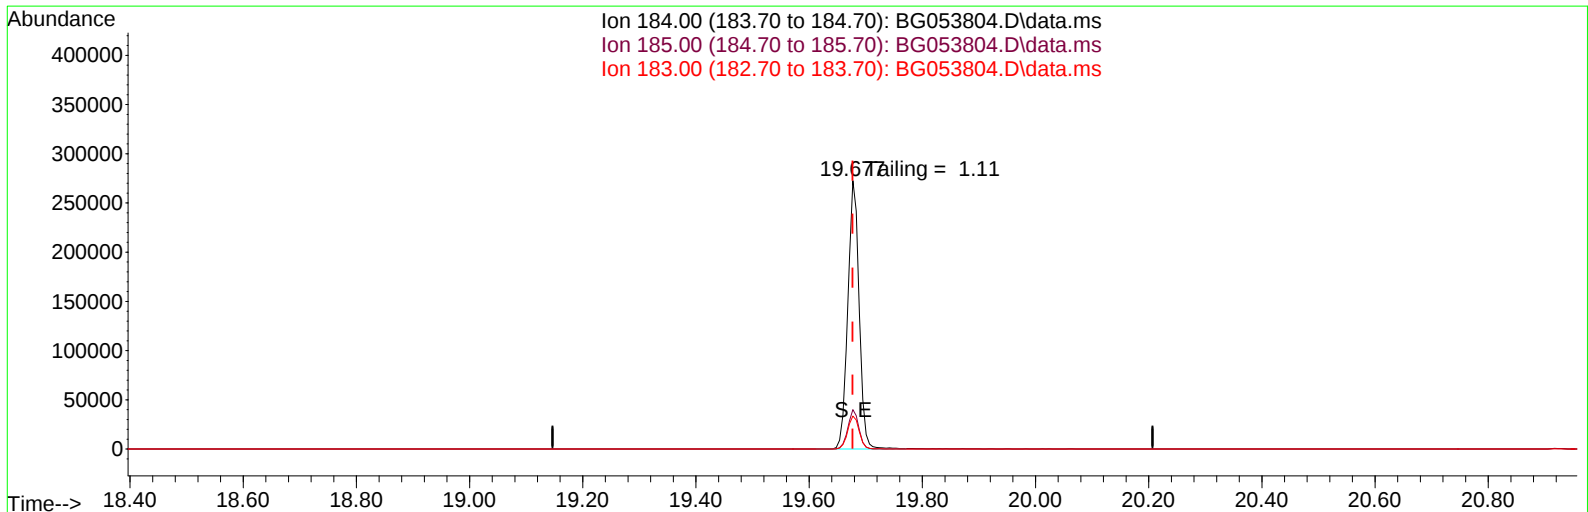

TIC: BG053804.D\data.ms

(77) Benzidine

19.677min (+ 0.001) 0.00 ng

response 379551

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.66
183.00	11.10	12.30
0.00	0.00	0.00