


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060419\
 Data File : BG041056.D
 Acq On : 4 Jun 2019 11:53
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

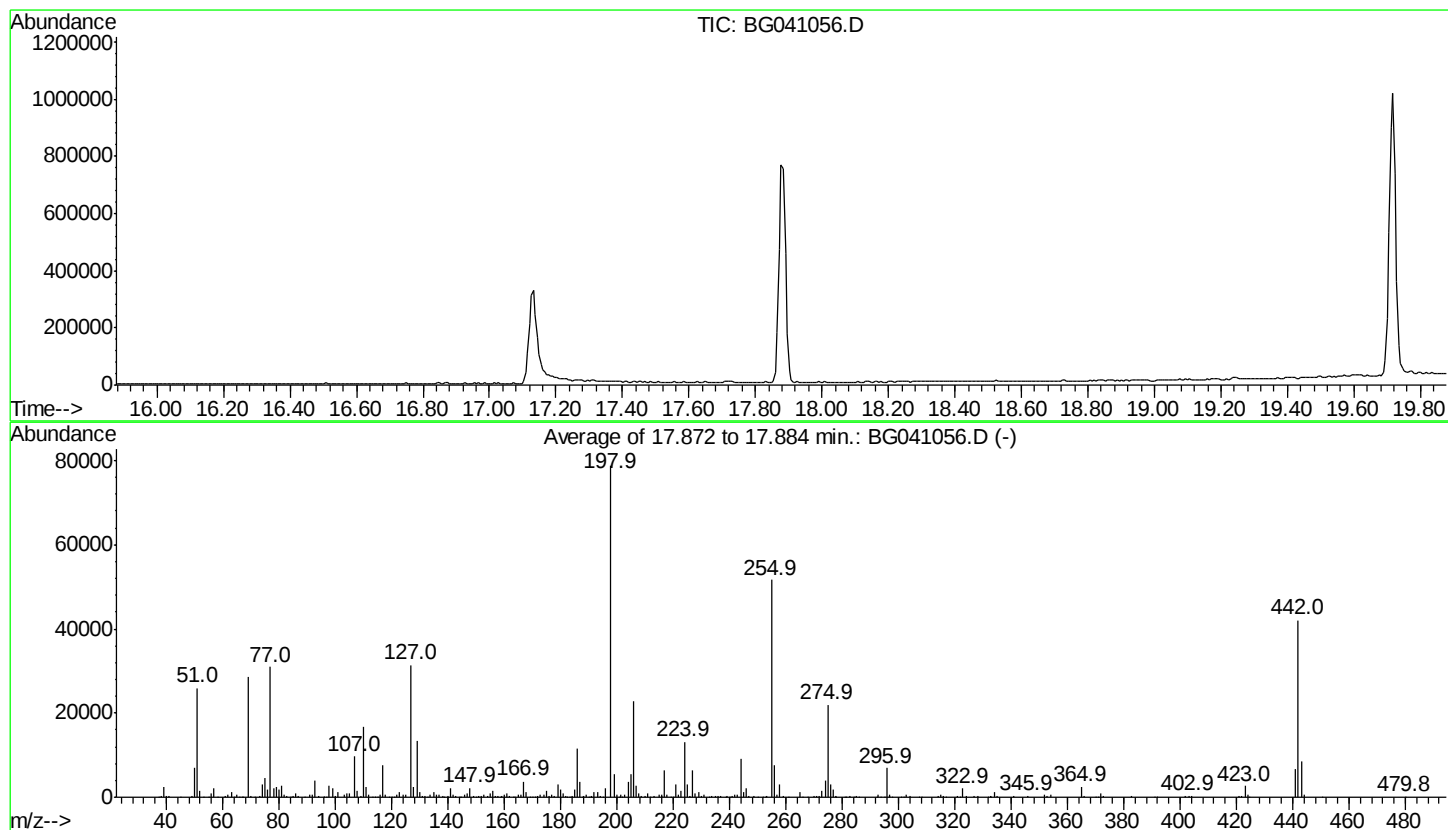

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	25991	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.1	28458	PASS
70	69	0.00	2	1.0	279	PASS
127	198	10	80	39.8	31349	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78805	PASS
199	198	5	9	7.1	5590	PASS
275	198	10	60	28.0	22046	PASS
365	198	1	100	3.1	2474	PASS
441	198	0.01	100	8.5	6723	PASS
442	198	50	100	53.3	42010	PASS
443	442	15	24	20.0	8417	PASS