

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
 Data File : BG041083.D
 Acq On : 6 Jun 2019 9:52
 Operator : HP/JU
 Sample : PB120328BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120328BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.646	429	435	447	rBV	706157	1151578	36.75%	7.509%
2	7.256	701	709	718	rBV	746296	1269902	40.52%	8.281%
3	7.637	767	774	783	rBV	731889	1232819	39.34%	8.039%
4	8.113	848	855	863	rBV	154118	266042	8.49%	1.735%
5	8.437	901	910	918	rBV	540288	941155	30.03%	6.137%
6	9.288	1047	1055	1066	rBV	444144	794085	25.34%	5.178%
7	10.934	1328	1335	1343	rBV	189396	344548	10.99%	2.247%
8	13.366	1742	1749	1763	rBV	1132595	1822741	58.16%	11.886%
9	14.741	1974	1983	1993	rBV2	298368	489901	15.63%	3.195%
10	16.227	2229	2236	2250	rBV	987855	1518246	48.45%	9.900%
11	17.485	2444	2450	2460	rBV2	442862	655533	20.92%	4.275%
12	20.082	2886	2892	2901	rBV	2509277	3133924	100.00%	20.436%
13	21.762	3171	3178	3187	rBV2	503762	858073	27.38%	5.595%
14	25.093	3729	3745	3757	rVB	284726	856741	27.34%	5.587%


Sum of corrected areas: 15335288

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
Data File : BG041083.D
Acq On : 6 Jun 2019 9:52
Operator : HP/JU
Sample : PB120328BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120328BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

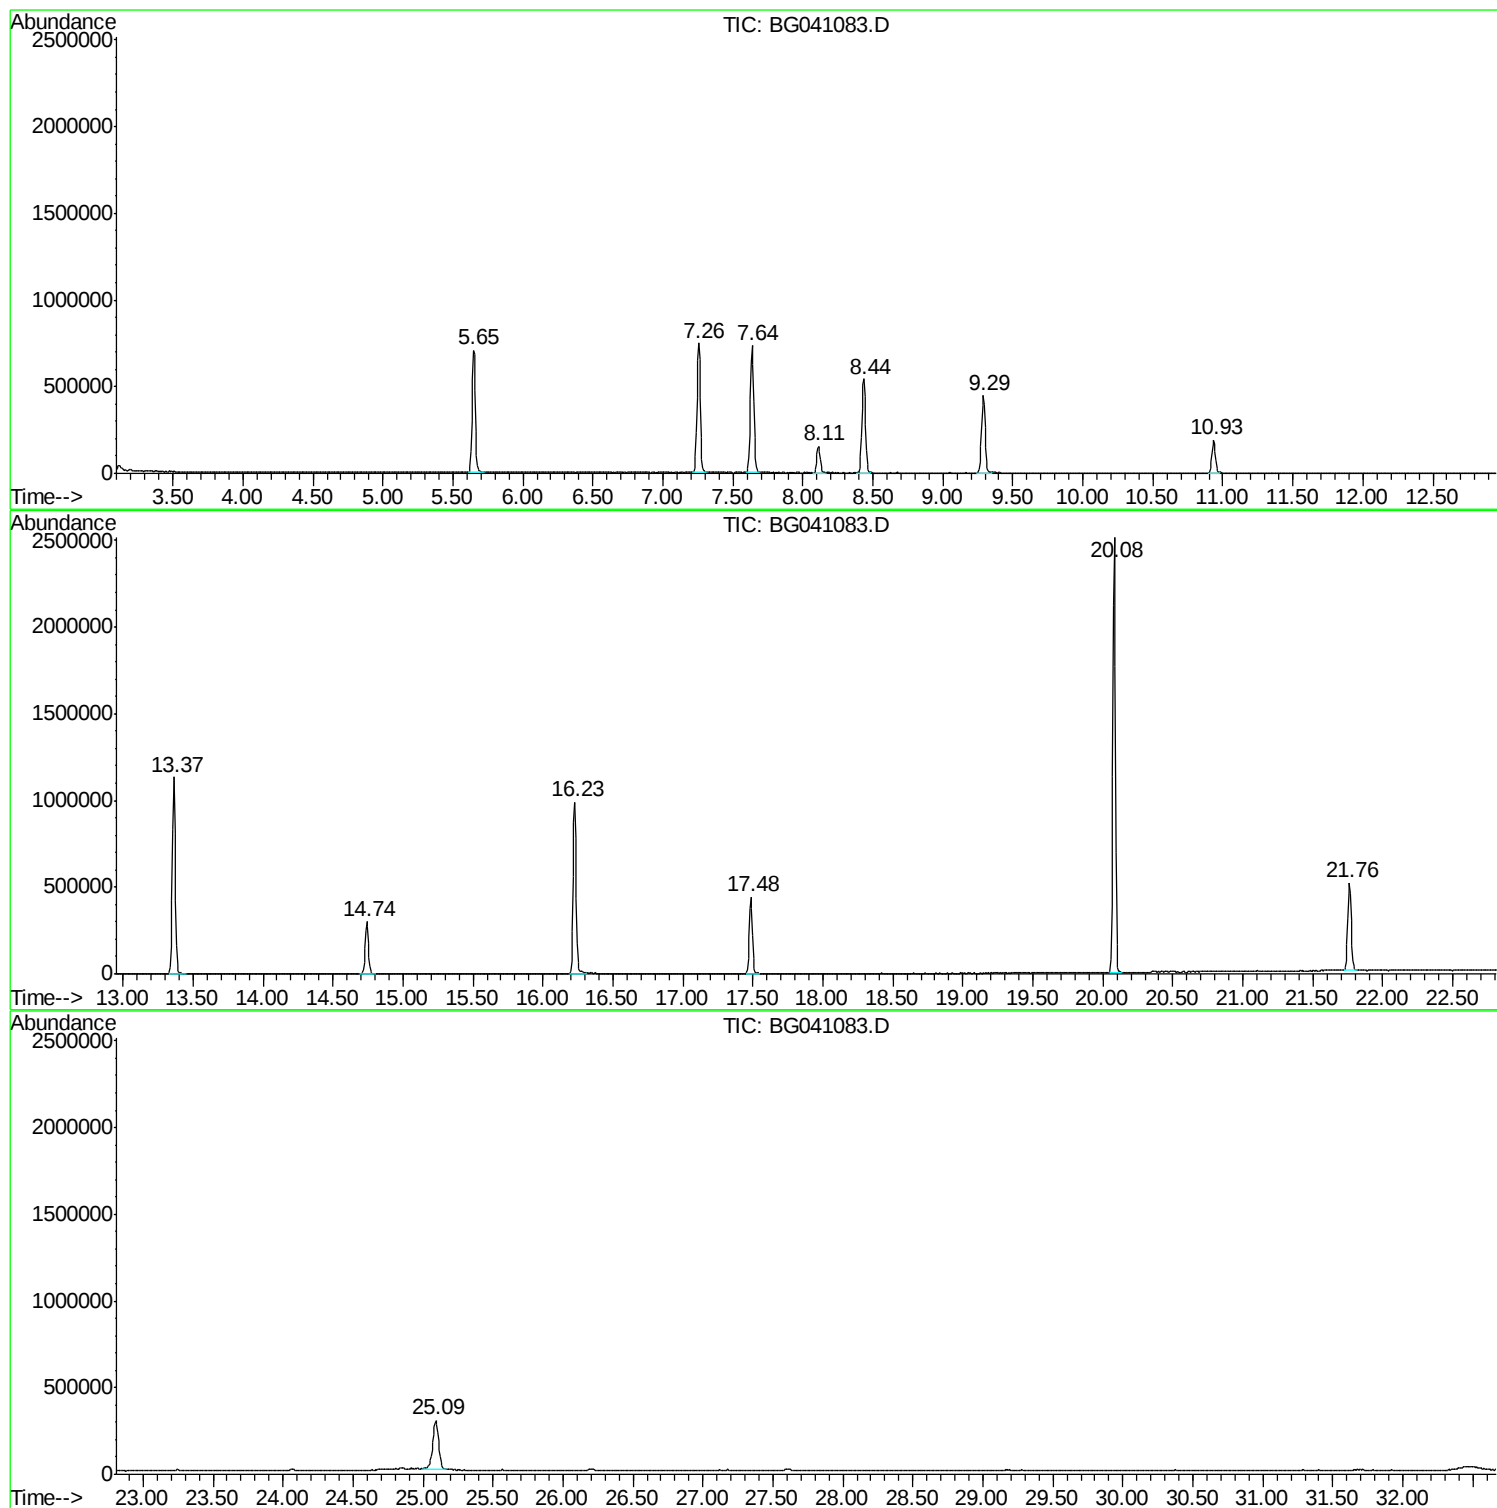

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
Data File : BG041083.D
Acq On : 6 Jun 2019 9:52
Operator : HP/JU
Sample : PB120328BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120328BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.64 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.64	92.68 ng	1232820	1,4-Dichlorobenzene-d4	8.11

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27		
2	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22		
3	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16		
4	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	13		
5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12		

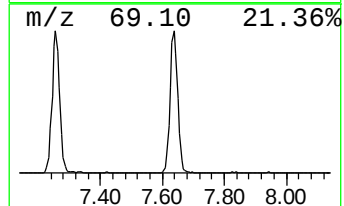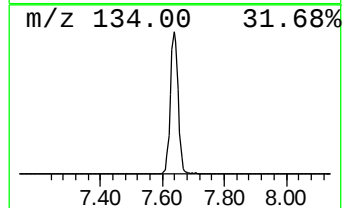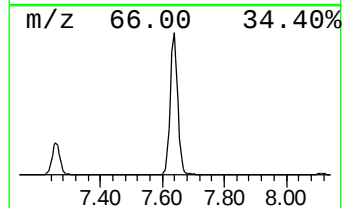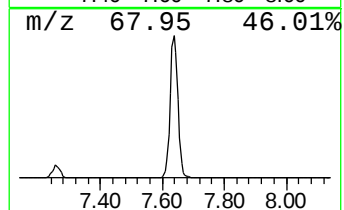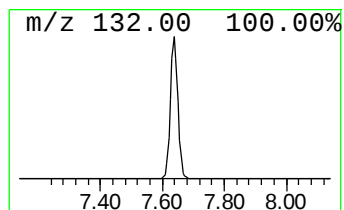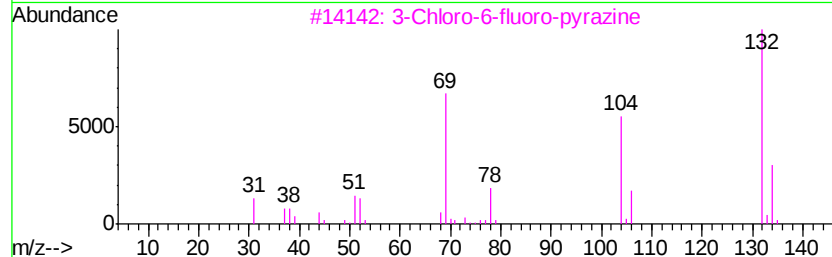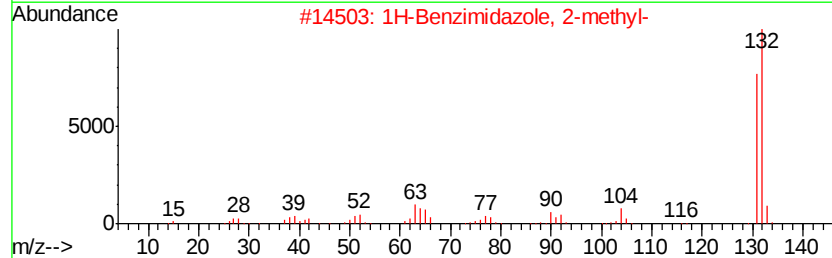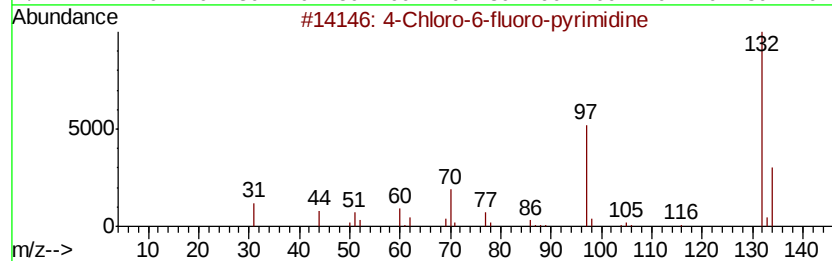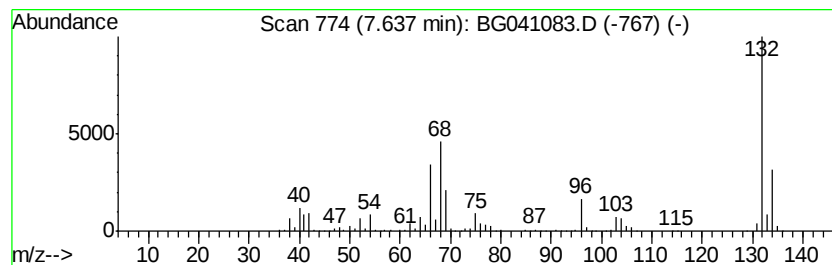

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060619\
Data File : BG041083.D
Acq On : 6 Jun 2019 9:52
Operator : HP/JU
Sample : PB120328BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120328BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.64	7.64	92.7	ng	1232820	1	8.11	266042	20.0