

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
 Data File : BG041088.D
 Acq On : 6 Jun 2019 13:03
 Operator : HP/JU
 Sample : PB120371BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120371BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.647	427	435	450	rBV	799105	1288684	37.57%	7.539%
2	7.257	701	709	721	rBV	825593	1402179	40.88%	8.203%
3	7.639	766	774	784	rBV	799764	1373280	40.03%	8.034%
4	8.114	847	855	863	rBV	177121	314911	9.18%	1.842%
5	8.438	902	910	924	rVB	599503	1050551	30.63%	6.146%
6	9.290	1047	1055	1064	rBV	482202	867175	25.28%	5.073%
7	10.935	1324	1335	1346	rBV	222349	409170	11.93%	2.394%
8	13.361	1741	1748	1759	rBV	1273036	1975977	57.60%	11.560%
9	14.742	1976	1983	1992	rBV2	347717	570301	16.63%	3.337%
10	16.229	2229	2236	2252	rBV	1056446	1654744	48.24%	9.681%
11	17.486	2443	2450	2459	rBV2	506409	762294	22.22%	4.460%
12	20.083	2886	2892	2899	rBV	2712498	3430243	100.00%	20.068%
13	21.763	3171	3178	3188	rBV	614110	993135	28.95%	5.810%
14	25.095	3731	3745	3761	rVB	329295	1000110	29.16%	5.851%


Sum of corrected areas: 17092754

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
Data File : BG041088.D
Acq On : 6 Jun 2019 13:03
Operator : HP/JU
Sample : PB120371BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120371BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

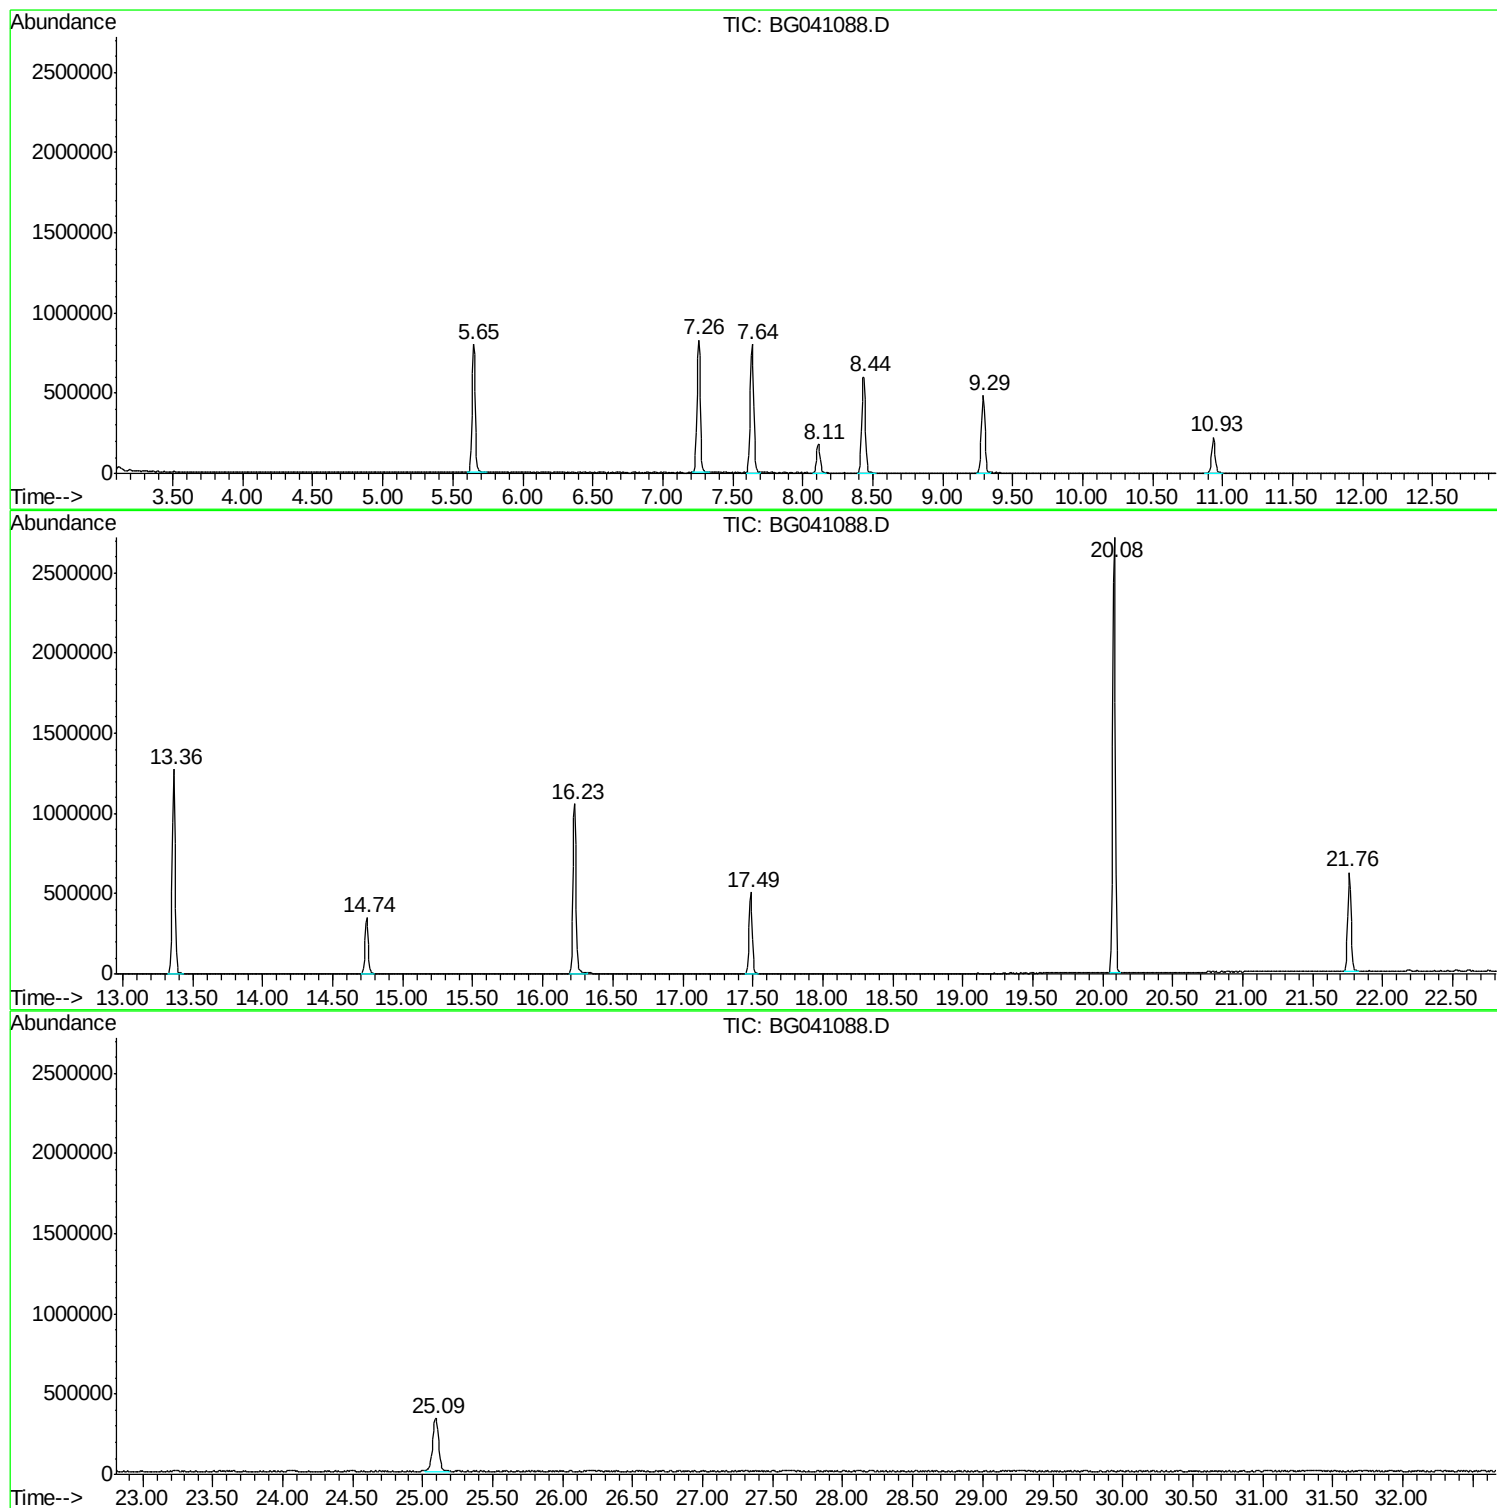

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
Data File : BG041088.D
Acq On : 6 Jun 2019 13:03
Operator : HP/JU
Sample : PB120371BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120371BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.64 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.64	87.22 ng	1373280	1,4-Dichlorobenzene-d4	8.11

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	12

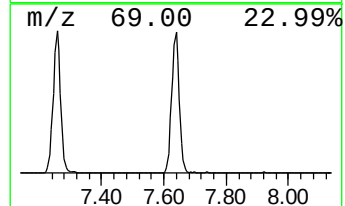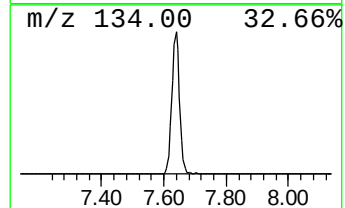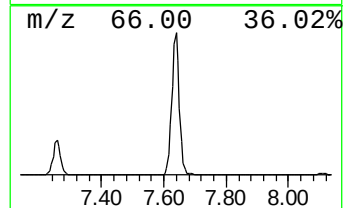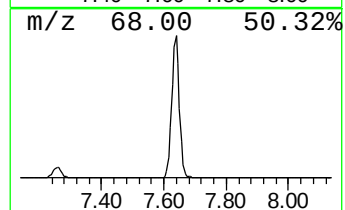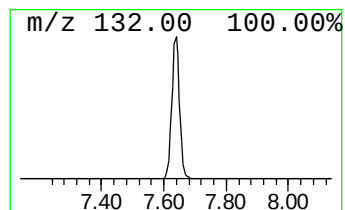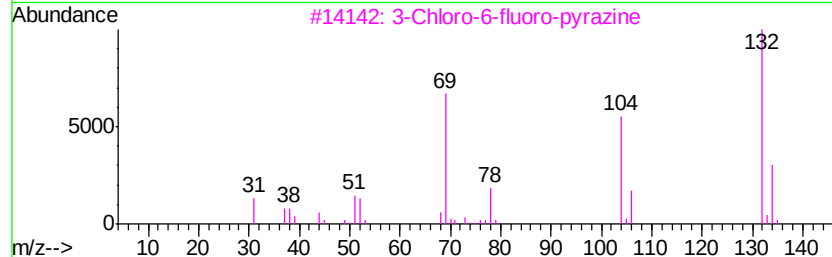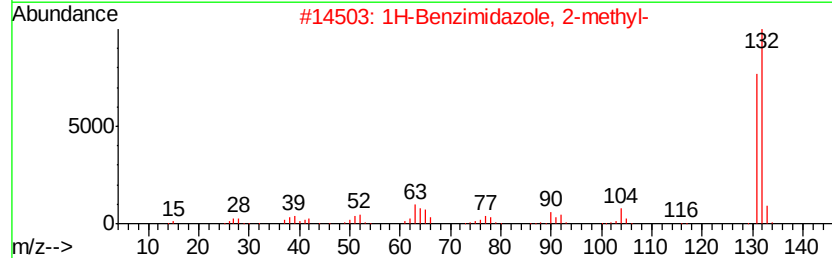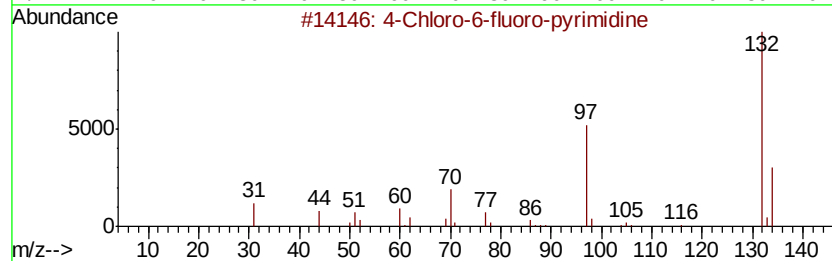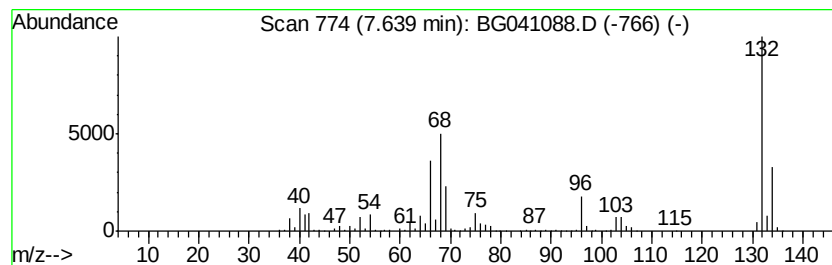

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060619\
Data File : BG041088.D
Acq On : 6 Jun 2019 13:03
Operator : HP/JU
Sample : PB120371BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120371BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.64	7.64	87.2	ng	1373280	1	8.11	314911	20.0