


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060619\
 Data File : BG041081.D
 Acq On : 6 Jun 2019 8:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 29 18:39:57 2019

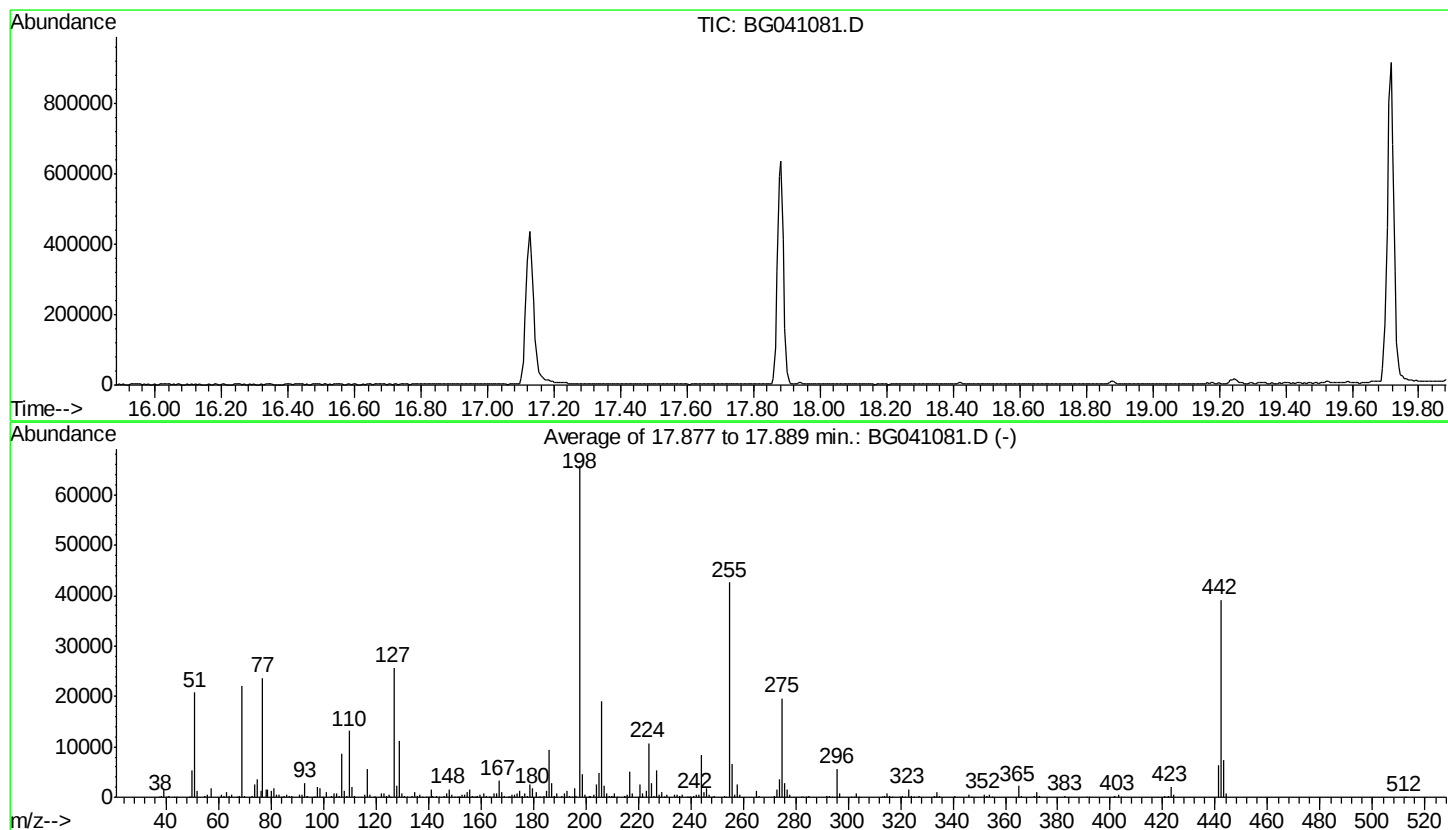

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	20804	PASS
68	69	0.00	2	1.1	235	PASS
69	198	0.00	100	33.7	22140	PASS
70	69	0.00	2	0.6	137	PASS
127	198	10	80	39.2	25765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65786	PASS
199	198	5	9	7.0	4585	PASS
275	198	10	60	29.9	19659	PASS
365	198	1	100	3.4	2259	PASS
441	198	0.01	100	9.6	6301	PASS
442	198	50	100	59.6	39184	PASS
443	442	15	24	18.9	7396	PASS