
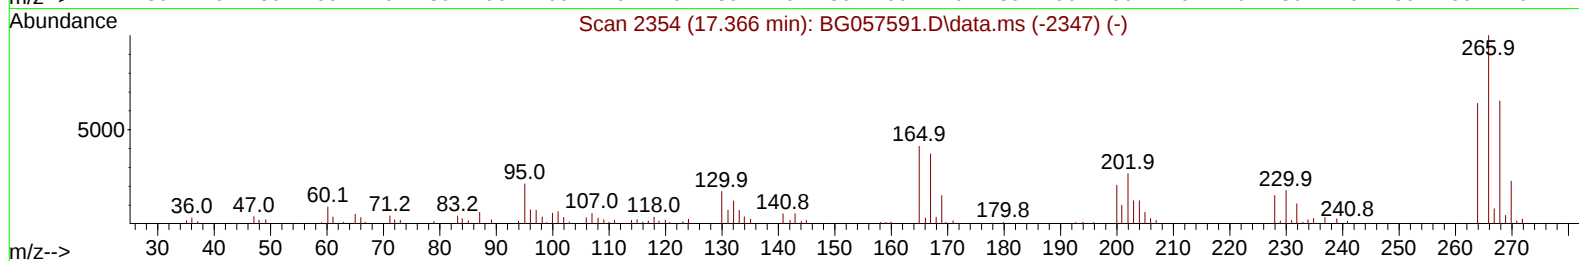
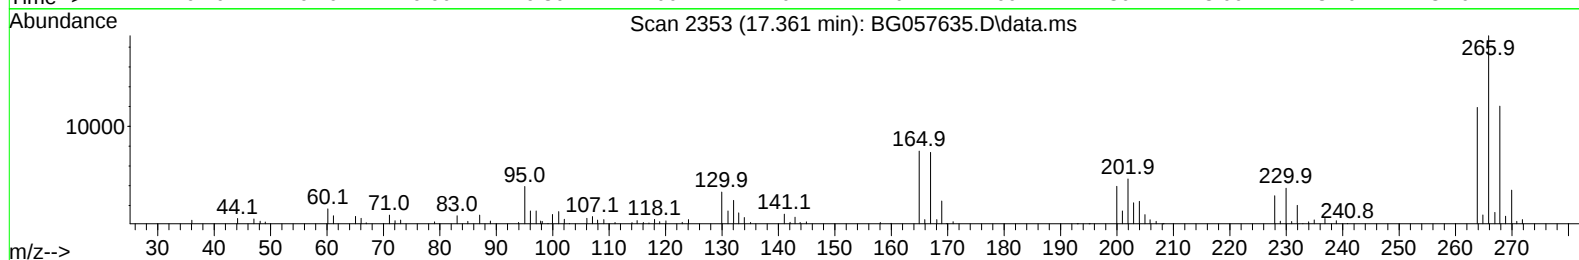


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057635.D
Acq On : 6 Jun 2023 12:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 13:33:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

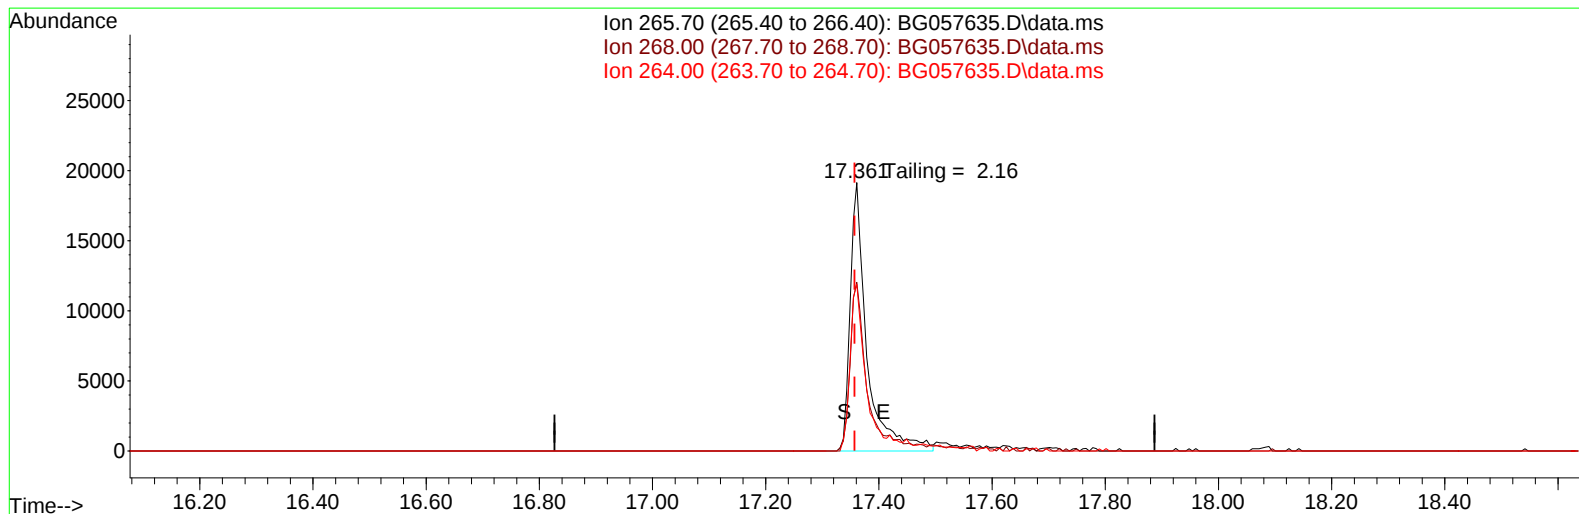

TIC: BG057635.D\data.ms

(70) Pentachlorophenol (C)




17.361min (+ 0.004) 23944.16 ng

response 39500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.86
264.00	64.00	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057635.D
Acq On : 6 Jun 2023 12:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 13:33:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

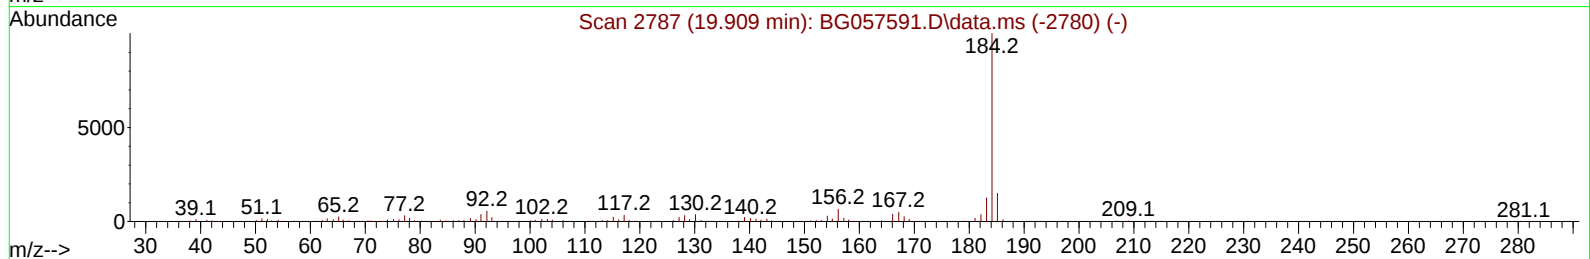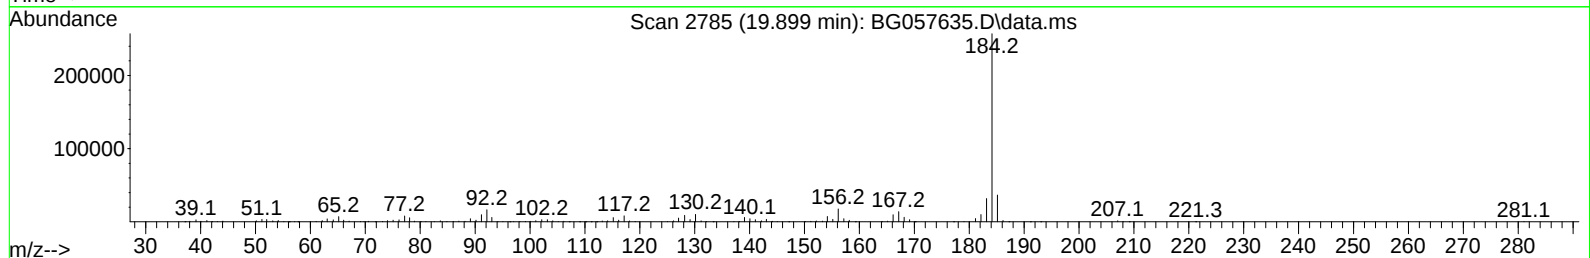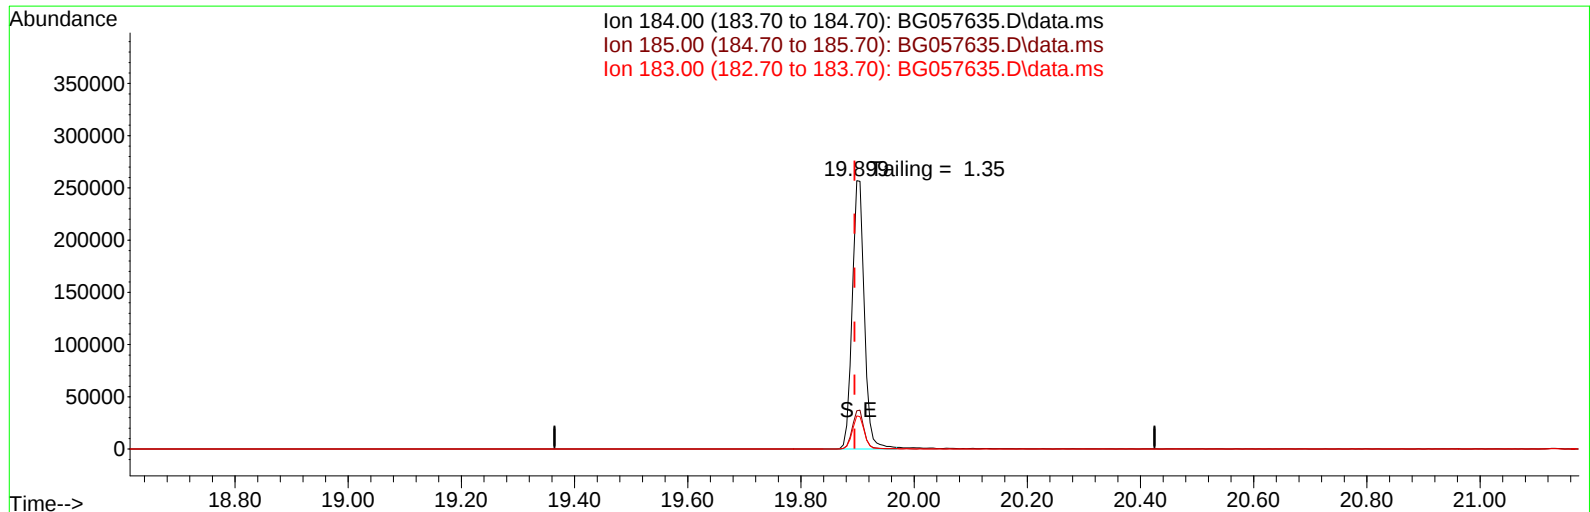

TIC: BG057635.D\data.ms

(77) Benzidine**19.899min (+ 0.004) 235001.07 ng****response 384003**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.27
183.00	12.50	12.38
0.00	0.00	0.00