

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
 Data File : BG057642.D
 Acq On : 6 Jun 2023 18:11
 Operator : CG/JU
 Sample : PB153157BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB153157BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.858	389	395	411	rBV	433241	728896	30.31%	6.872%
2	7.491	666	673	689	rBV	453145	807240	33.56%	7.610%
3	8.337	811	817	827	rVB	145258	251820	10.47%	2.374%
4	9.524	1010	1019	1036	rBV	260382	490968	20.41%	4.629%
5	11.180	1292	1301	1316	rBV	202078	373286	15.52%	3.519%
6	13.583	1703	1710	1719	rBV	888436	1328240	55.23%	12.522%
7	14.957	1937	1944	1952	rBV	374270	592494	24.64%	5.586%
8	16.444	2190	2197	2213	rBV	650147	1039363	43.22%	9.799%
9	17.701	2404	2411	2420	rBV	539074	833277	34.65%	7.856%
10	20.268	2842	2848	2854	rBV	1781633	2405055	100.00%	22.674%
11	22.001	3136	3143	3151	rBV	492779	878458	36.53%	8.282%
12	25.496	3727	3738	3750	rVB	302819	877880	36.50%	8.276%




Sum of corrected areas: 10606977

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057642.D
Acq On : 6 Jun 2023 18:11
Operator : CG/JU
Sample : PB153157BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153157BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

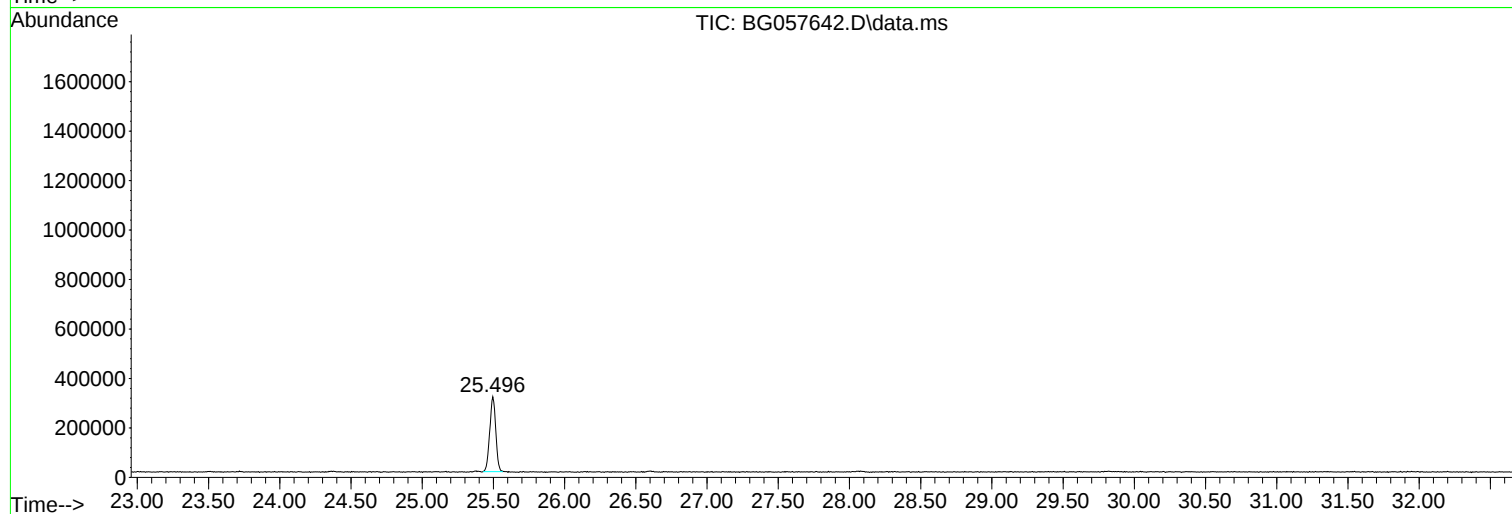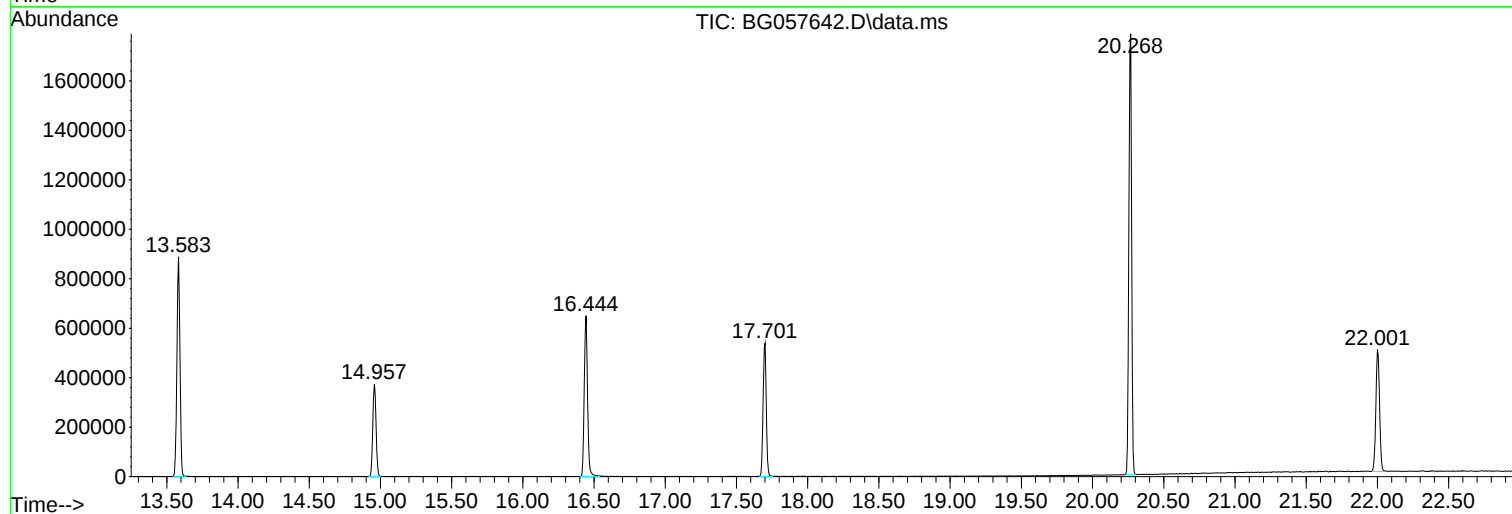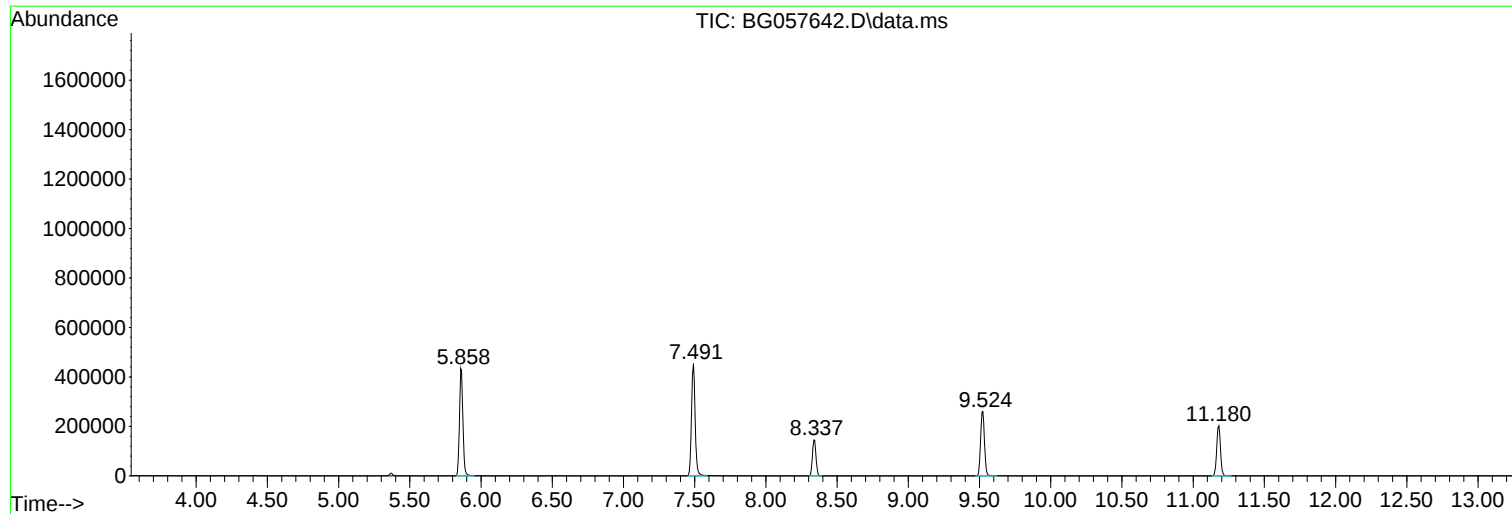

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057642.D
Acq On : 6 Jun 2023 18:11
Operator : CG/JU
Sample : PB153157BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153157BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057642.D
Acq On : 6 Jun 2023 18:11
Operator : CG/JU
Sample : PB153157BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153157BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------