

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
 Data File : BG057653.D
 Acq On : 7 Jun 2023 2:31
 Operator : CG/JU
 Sample : PB153181BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB153181BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.362	305	310	319	rBV	34986	53101	2.08%	0.583%
2	5.855	388	394	414	rBV	471235	763900	29.97%	8.385%
3	7.489	664	672	689	rBV	469702	843994	33.11%	9.264%
4	8.334	810	816	826	rBV	70998	121462	4.77%	1.333%
5	9.515	1009	1017	1028	rBV	275675	513987	20.17%	5.642%
6	11.178	1291	1300	1313	rVB	99751	182963	7.18%	2.008%
7	13.580	1702	1709	1725	rBV	882560	1401797	55.00%	15.386%
8	14.955	1936	1943	1952	rBV	182890	291392	11.43%	3.198%
9	16.441	2189	2196	2214	rBV	654757	1084139	42.54%	11.900%
10	17.692	2403	2409	2420	rBV	269236	413620	16.23%	4.540%
11	20.265	2840	2847	2854	rBV	1983995	2548776	100.00%	27.976%
12	21.998	3135	3142	3153	rVB2	253332	455254	17.86%	4.997%
13	25.488	3726	3736	3748	rVB	145275	436233	17.12%	4.788%




Sum of corrected areas: 9110618

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057653.D
Acq On : 7 Jun 2023 2:31
Operator : CG/JU
Sample : PB153181BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153181BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

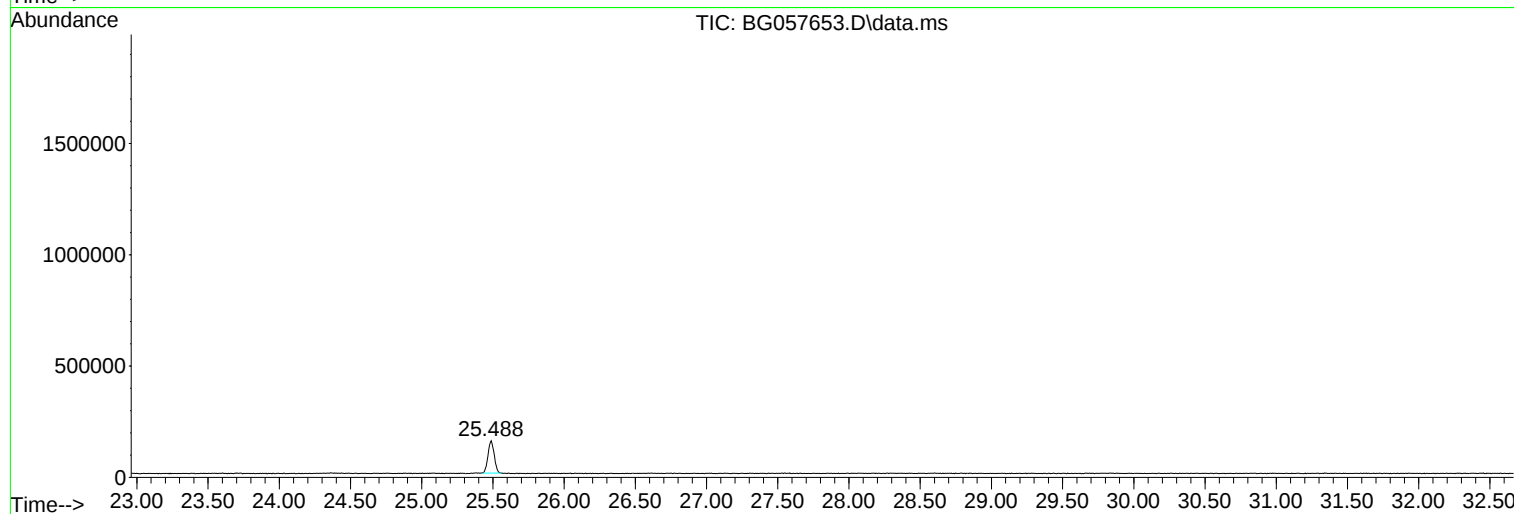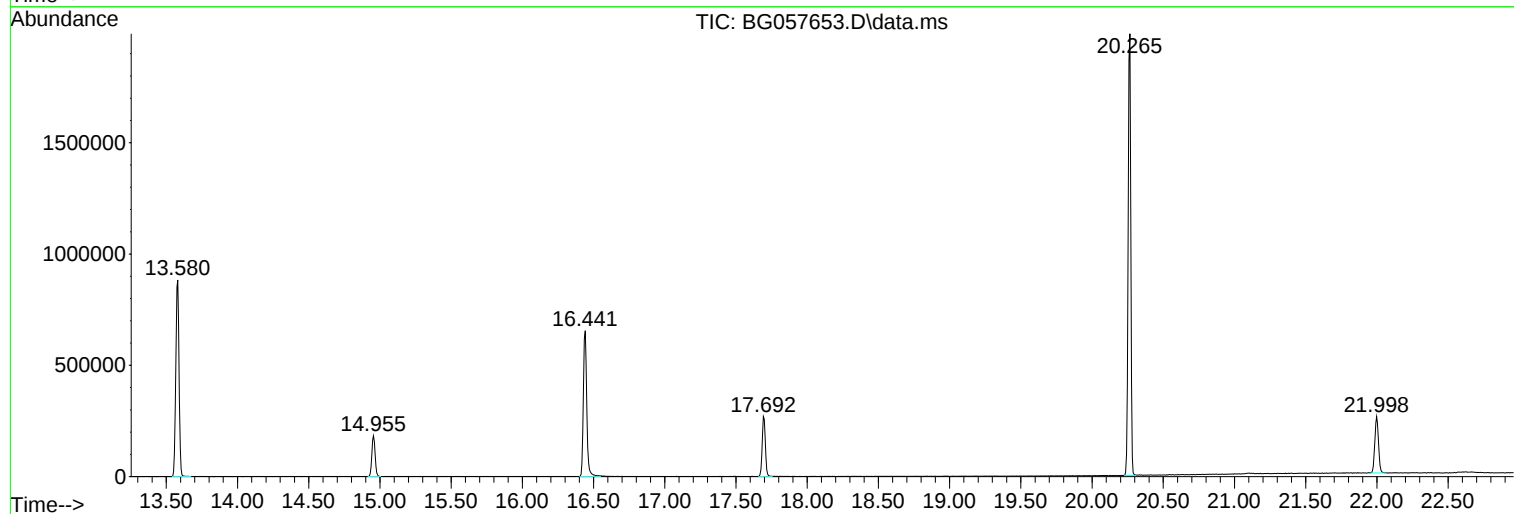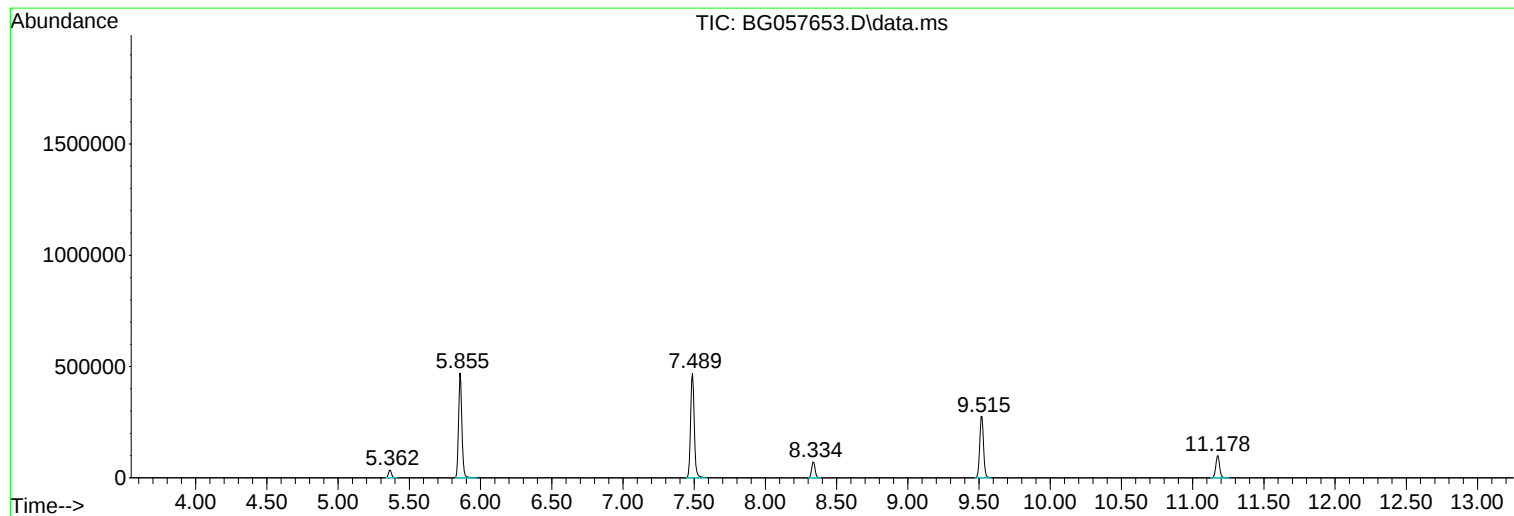

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057653.D
Acq On : 7 Jun 2023 2:31
Operator : CG/JU
Sample : PB153181BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153181BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.362	8.74 ng	53101	1,4-Dichlorobenzene-d4	8.340

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	38		
4	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	32		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		

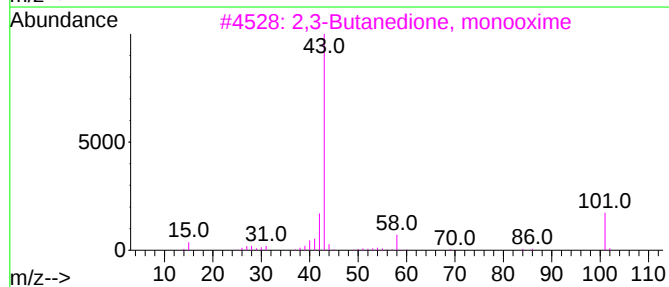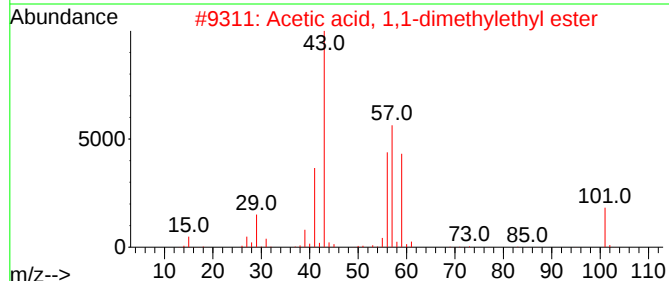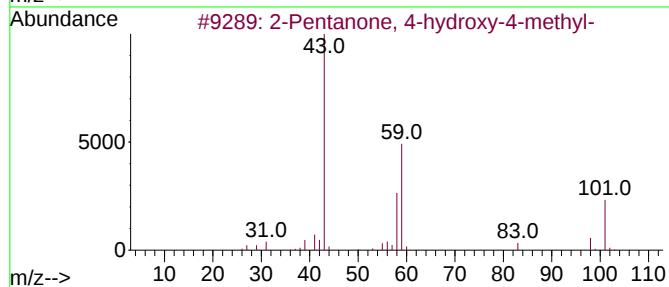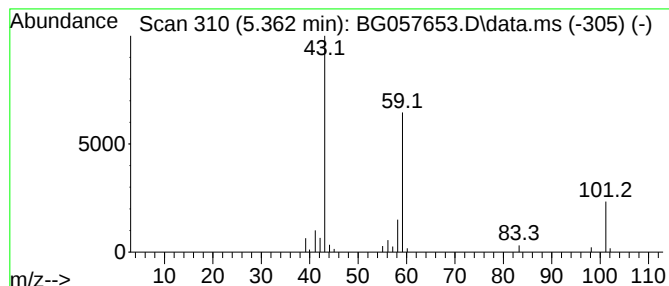

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057653.D
Acq On : 7 Jun 2023 2:31
Operator : CG/JU
Sample : PB153181BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153181BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.362	8.7	ng	53101	1	8.340	121462	20.0