

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057659.D
Acq On : 7 Jun 2023 6:39
Operator : CG/JU
Sample : PB153141BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153141BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.365	305	311	321	rVB	48449	75707	2.82%	0.760%
2	5.859	388	395	410	rBV	468170	781655	29.14%	7.851%
3	7.486	665	672	686	rBV	498351	881033	32.85%	8.849%
4	8.338	811	817	824	rBV	83670	140774	5.25%	1.414%
5	9.518	1010	1018	1030	rBV	297948	540864	20.16%	5.432%
6	11.175	1293	1300	1310	rBV	120242	221925	8.27%	2.229%
7	13.577	1702	1709	1726	rBV	1001904	1530905	57.07%	15.376%
8	14.952	1937	1943	1952	rBV	230356	367371	13.70%	3.690%
9	16.438	2190	2196	2215	rBV	720732	1161568	43.31%	11.666%
10	17.695	2403	2410	2423	rBV	336667	503778	18.78%	5.060%
11	20.263	2841	2847	2853	rBV	2082505	2682283	100.00%	26.940%
12	22.001	3136	3143	3151	rVB2	302621	537737	20.05%	5.401%
13	25.485	3726	3736	3749	rVB2	171686	530863	19.79%	5.332%




Sum of corrected areas: 9956463

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057659.D
Acq On : 7 Jun 2023 6:39
Operator : CG/JU
Sample : PB153141BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153141BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

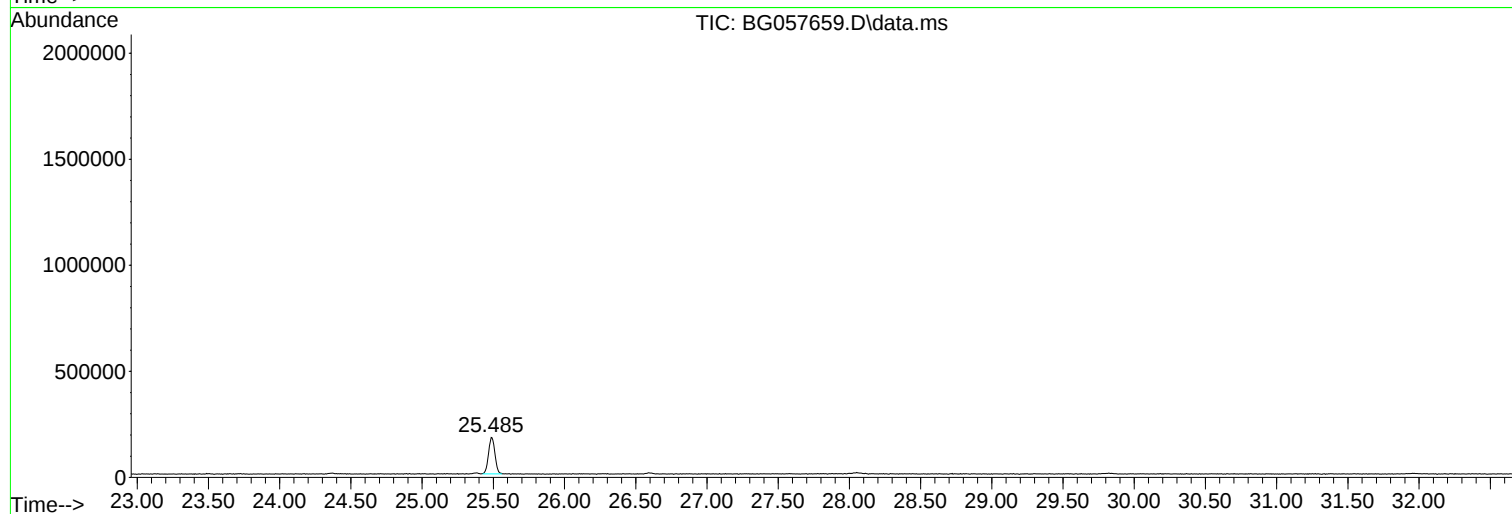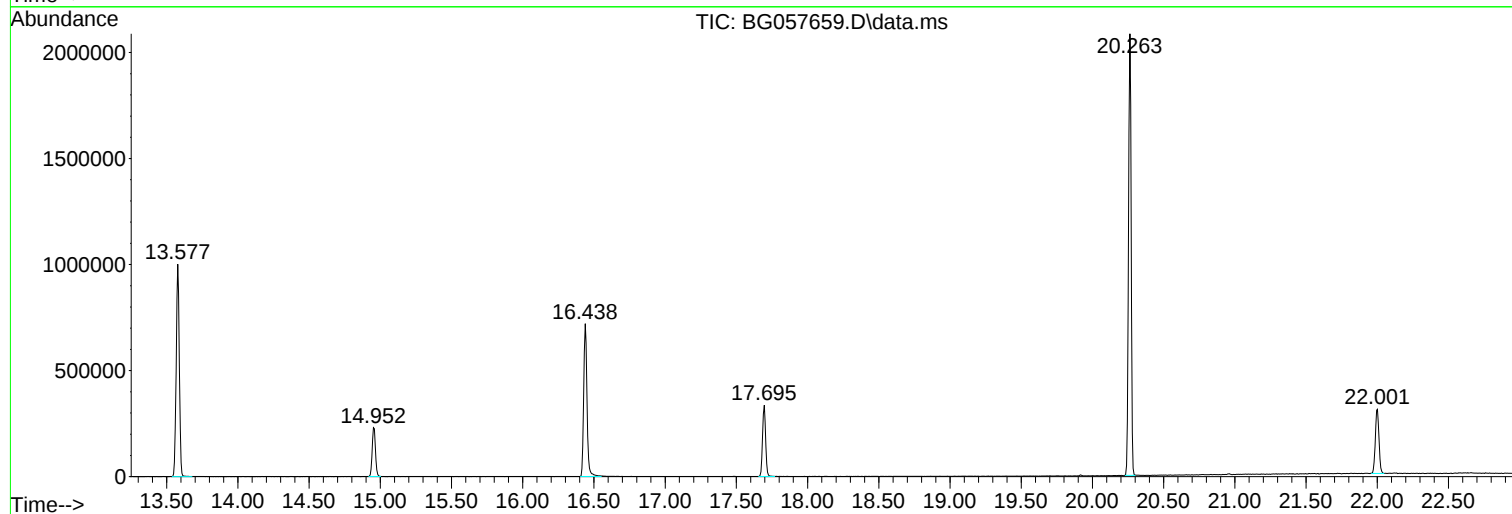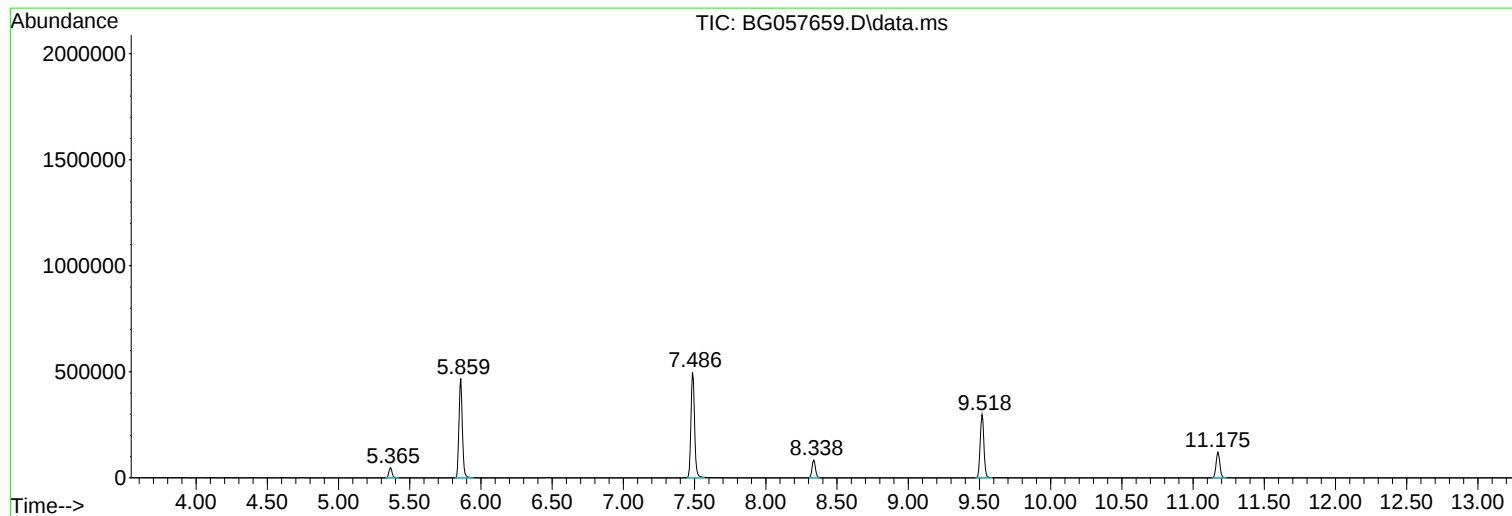

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057659.D
Acq On : 7 Jun 2023 6:39
Operator : CG/JU
Sample : PB153141BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153141BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.365	10.76 ng	75707	1,4-Dichlorobenzene-d4	8.338

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	25		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
4	Acetone	58	C3H6O	000067-64-1	14		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		

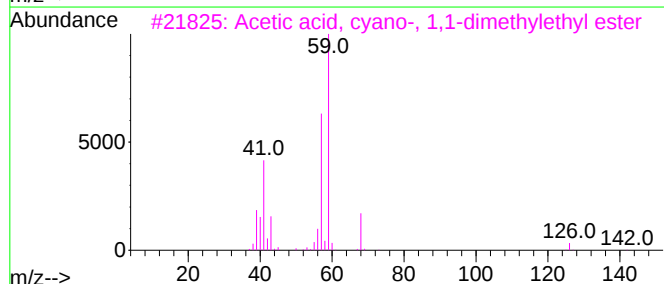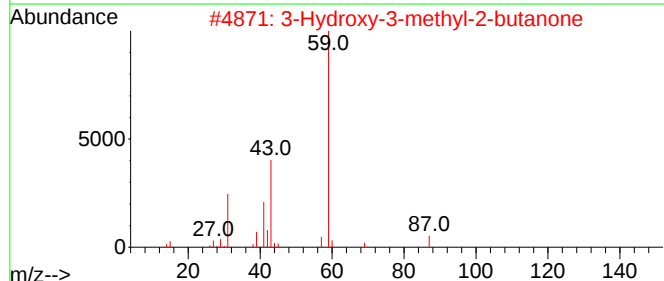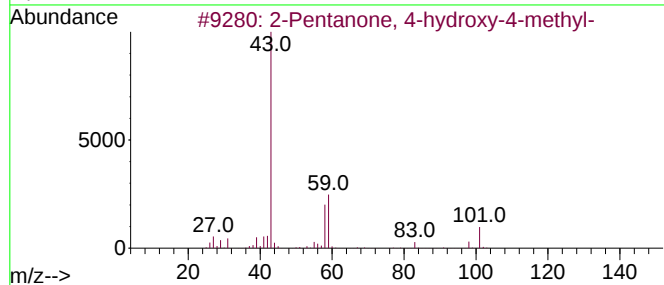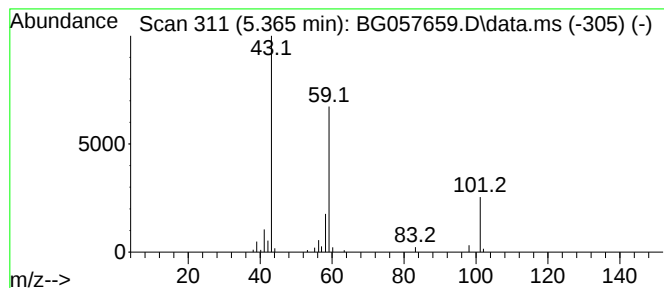

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057659.D
Acq On : 7 Jun 2023 6:39
Operator : CG/JU
Sample : PB153141BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153141BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.365	10.8	ng	75707	1	8.338	140774	20.0