
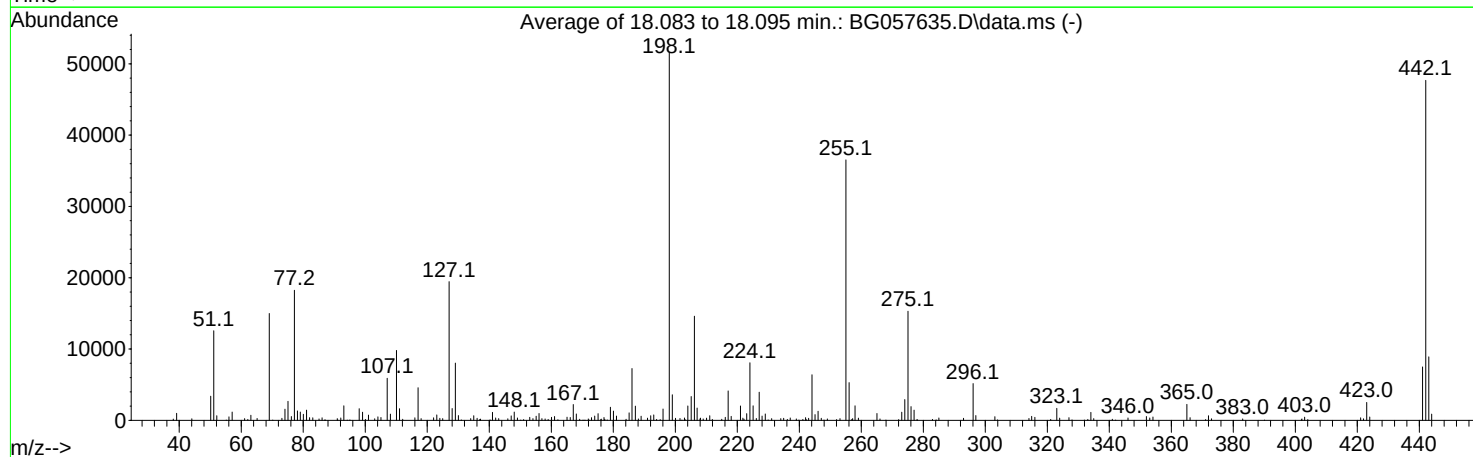


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
 Data File : BG057635.D
 Acq On : 6 Jun 2023 12:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 01 03:51:58 2023

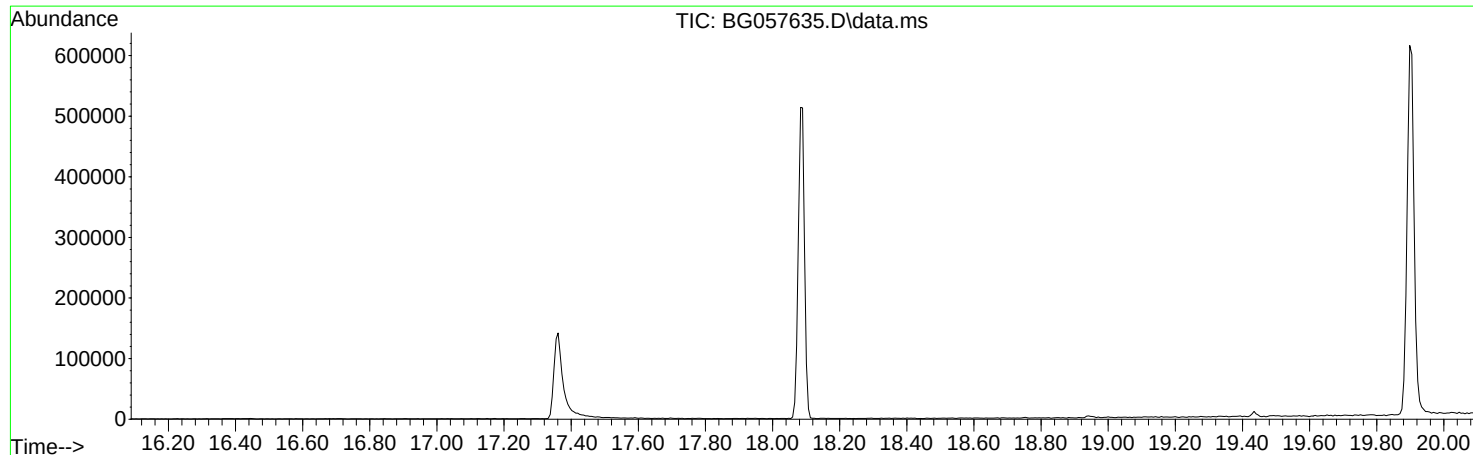

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.3	12560	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.1	14999	PASS
70	69	0.00	2	0.4	55	PASS
127	198	10	80	37.7	19462	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51584	PASS
199	198	5	9	7.0	3590	PASS
275	198	10	60	29.6	15294	PASS
365	198	1	100	4.4	2252	PASS
441	198	0.01	100	14.5	7493	PASS
442	442	50	100	100.0	47688	PASS
443	442	15	24	18.7	8906	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_G	<u>BG057635.D</u>
Compound Name	Response	Retention Time
DDT	174561	21.132
DDD	4972	20.68
DDE	219	20.175
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5191	179752	2.89

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057635.D
Acq On : 6 Jun 2023 12:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 06 13:33:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

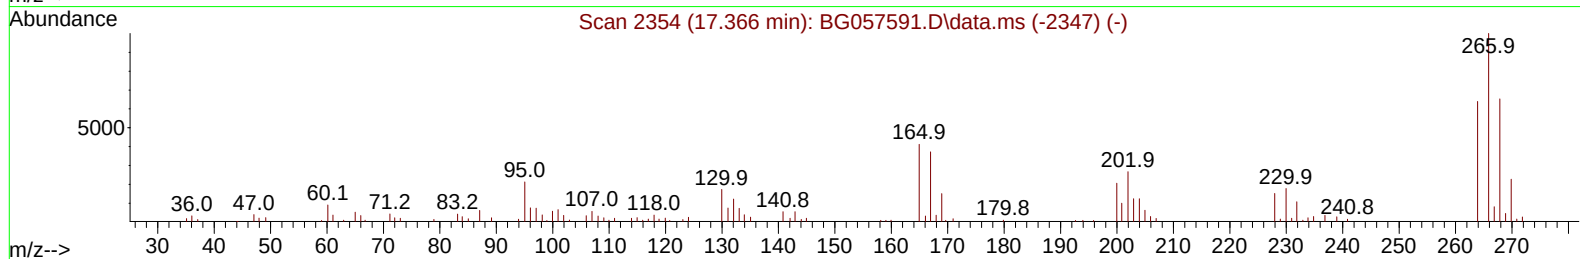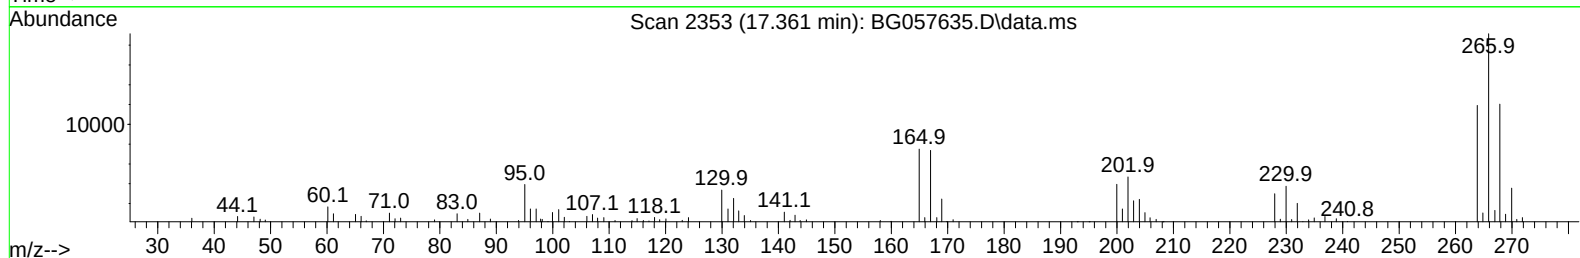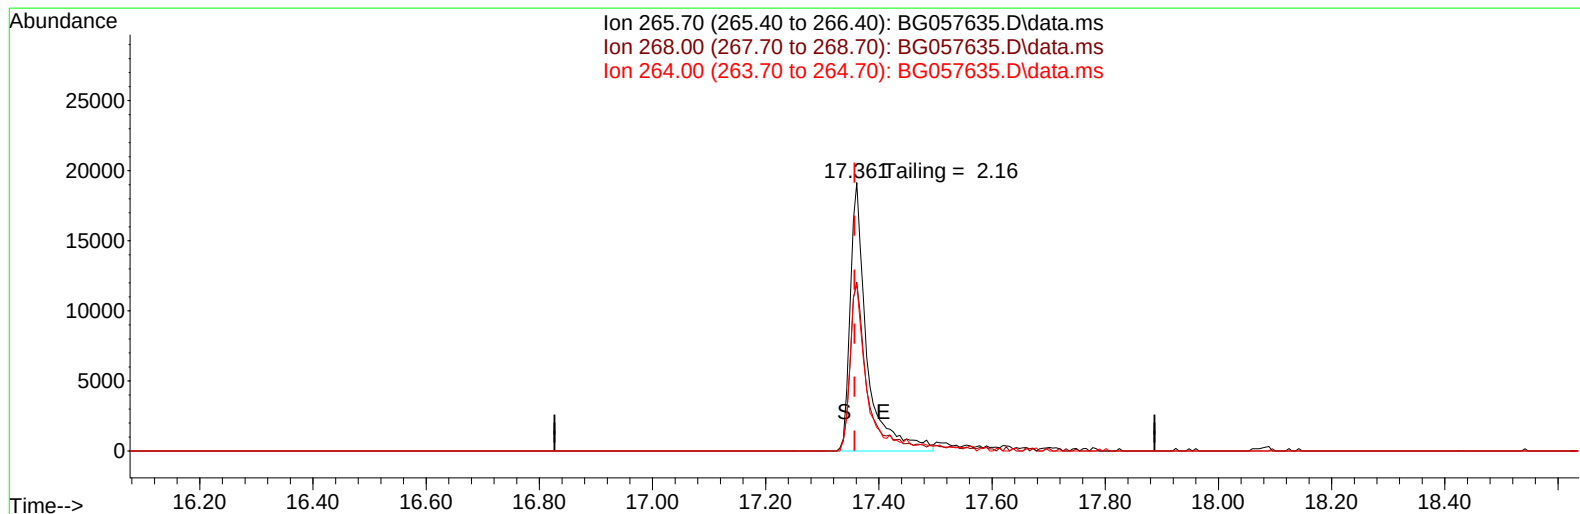

TIC: BG057635.D\data.ms

(70) Pentachlorophenol (C)

17.361min (+ 0.004) 23944.16 ng




response 39500

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.86
264.00	64.00	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057635.D
Acq On : 6 Jun 2023 12:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 06 13:33:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

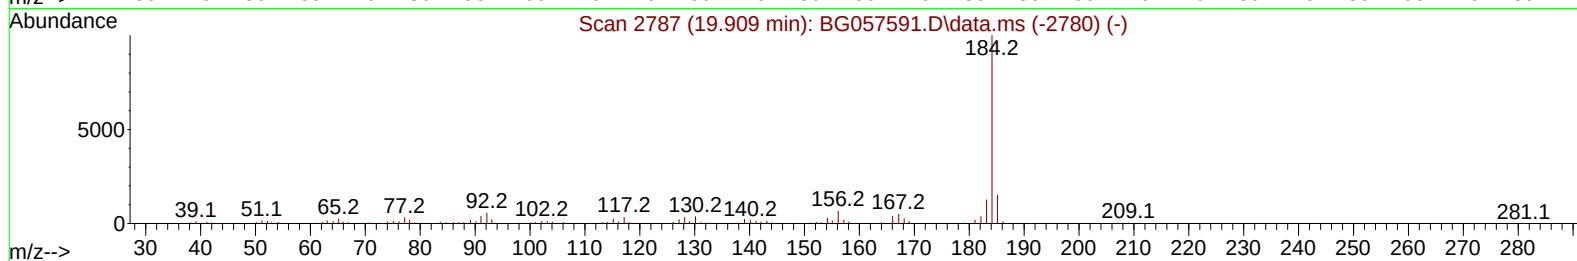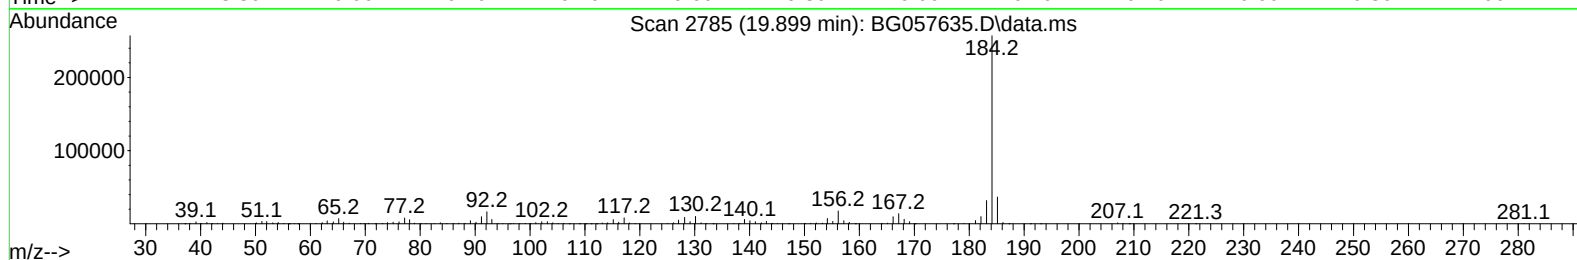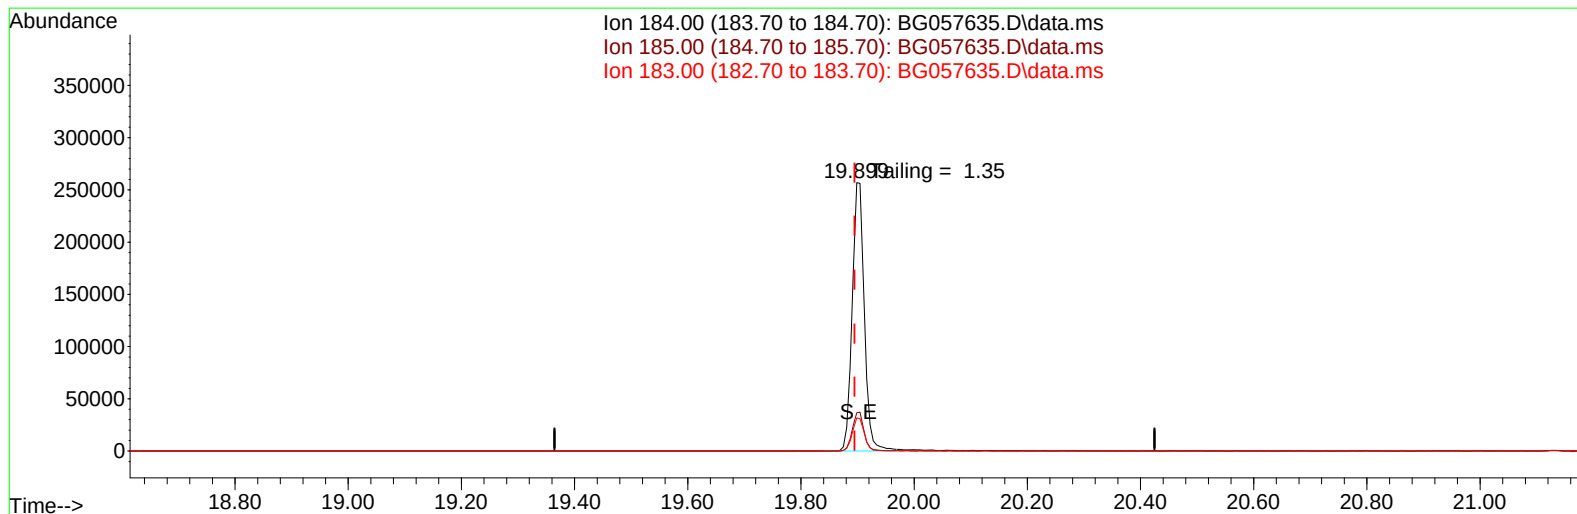

TIC: BG057635.D\data.ms

(77) Benzidine

19.899min (+ 0.004) 235001.07 ng

response 384003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.27
183.00	12.50	12.38
0.00	0.00	0.00