
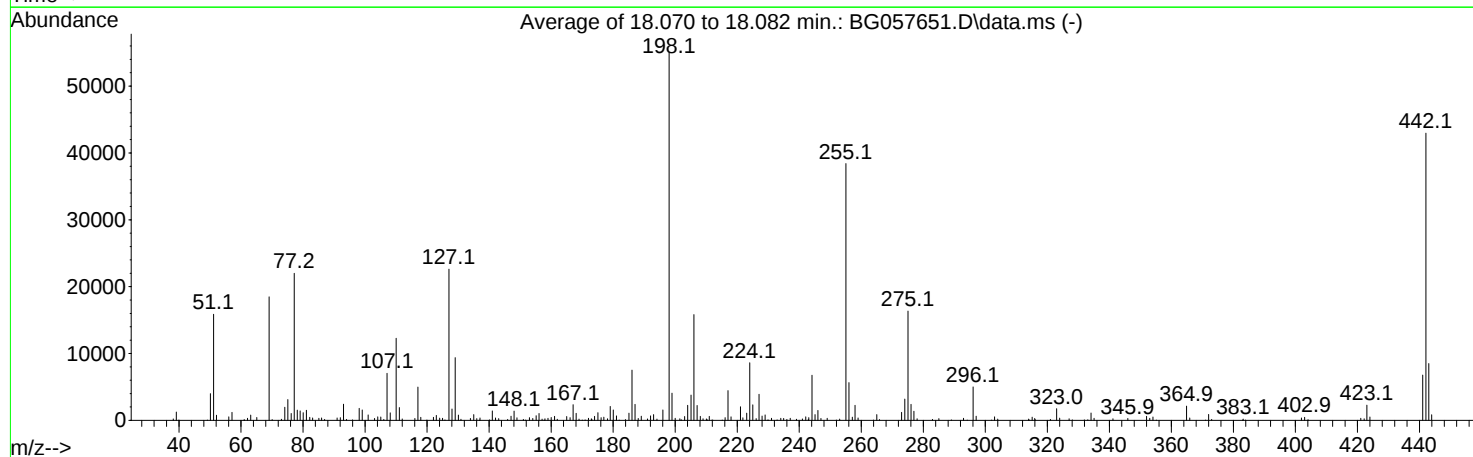


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057651.D
Acq On : 7 Jun 2023 1:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 01 03:51:58 2023

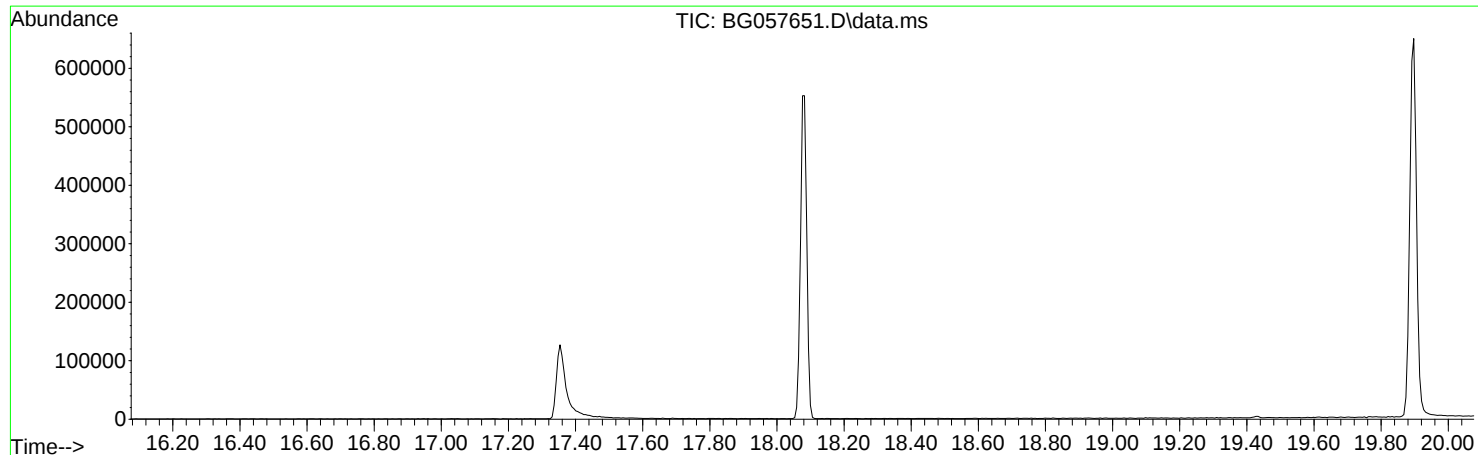

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	15870	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.6	18477	PASS
70	69	0.00	2	0.7	130	PASS
127	198	10	80	41.1	22611	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55027	PASS
199	198	5	9	7.4	4059	PASS
275	198	10	60	29.7	16349	PASS
365	198	1	100	3.9	2135	PASS
441	198	0.01	100	12.3	6786	PASS
442	442	50	100	100.0	42963	PASS
443	442	15	24	19.8	8492	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/6/2023	BNA_G	<u>BG057651.D</u>
Compound Name	Response	Retention Time
DDT	176744	21.119
DDD	11507	20.667
DDE	1541	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13048	189792	6.87

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057651.D
Acq On : 7 Jun 2023 1:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 07 07:39:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

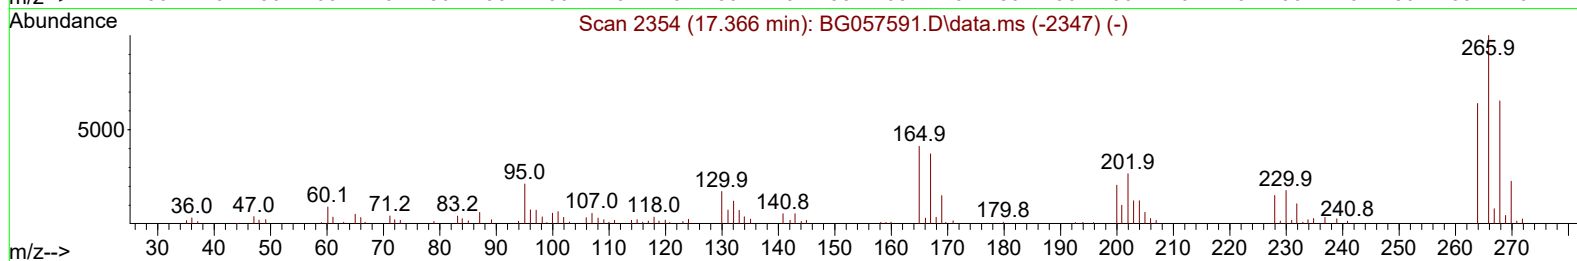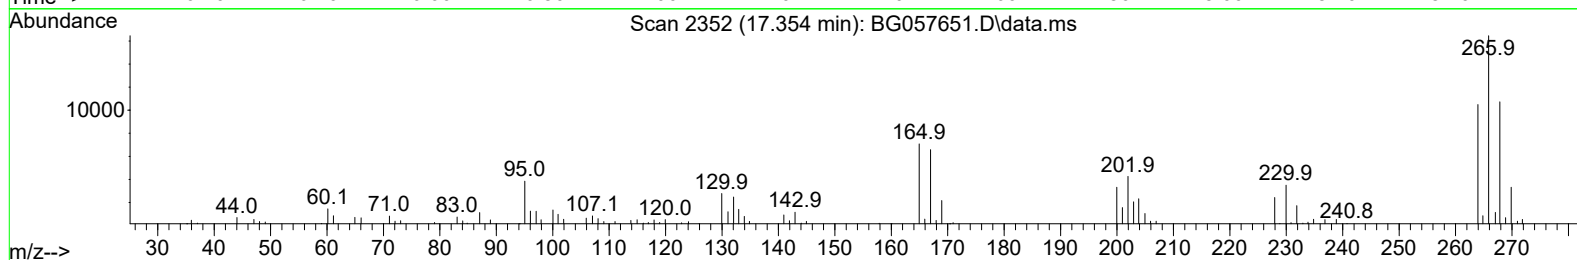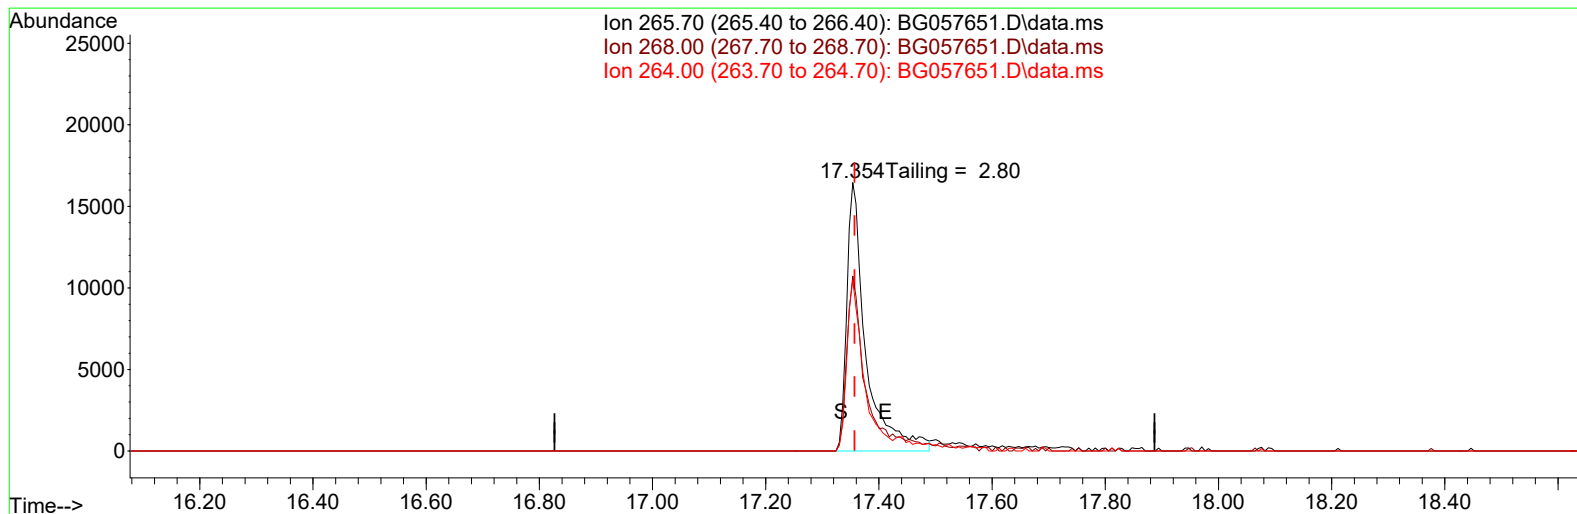

TIC: BG057651.D\data.ms

(70) Pentachlorophenol (C)

17.354min (-0.003) 17328.06 ng




response 36855

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.17
264.00	64.00	63.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060623\
Data File : BG057651.D
Acq On : 7 Jun 2023 1:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 07 07:39:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

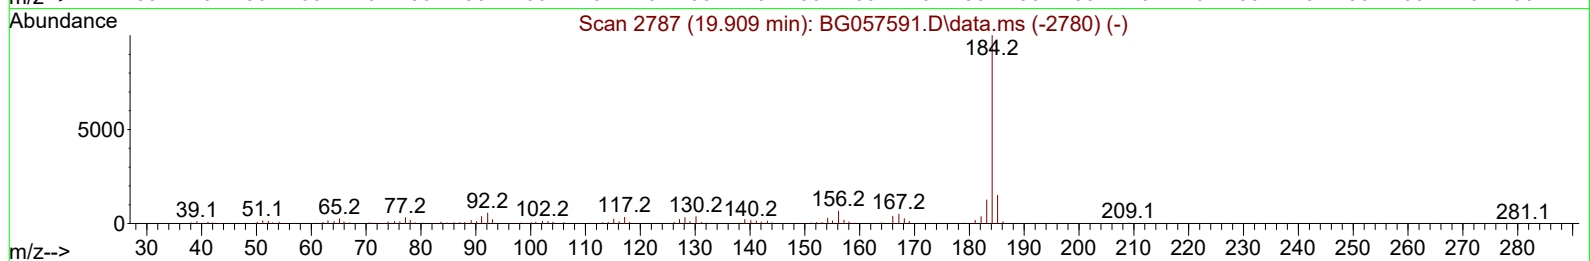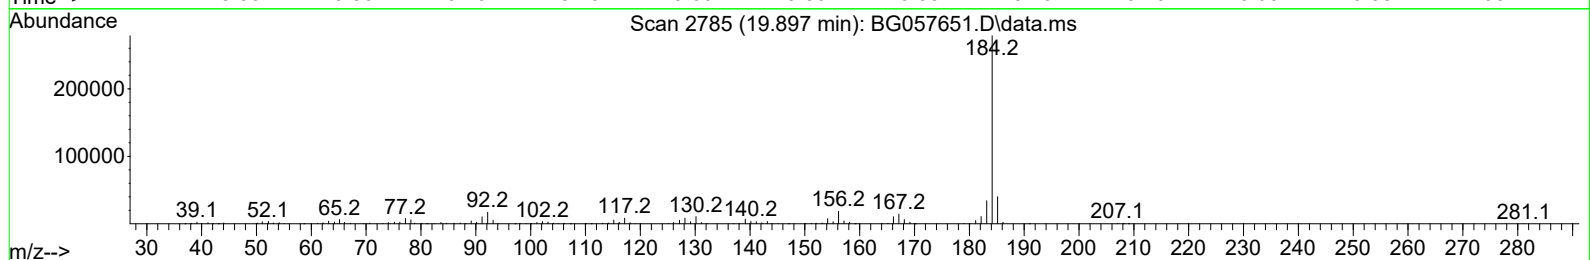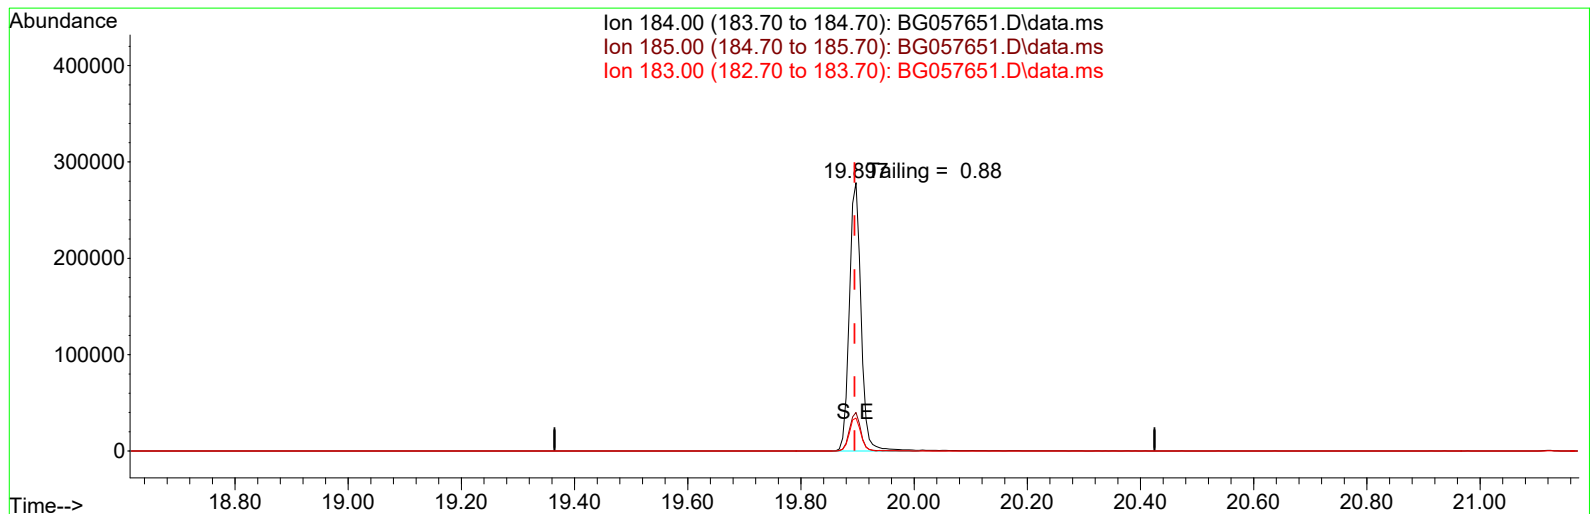

TIC: BG057651.D\data.ms

(77) Benzidine

19.897min (+ 0.003) 0.00 ng

response 397461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.41
183.00	12.50	12.29
0.00	0.00	0.00