
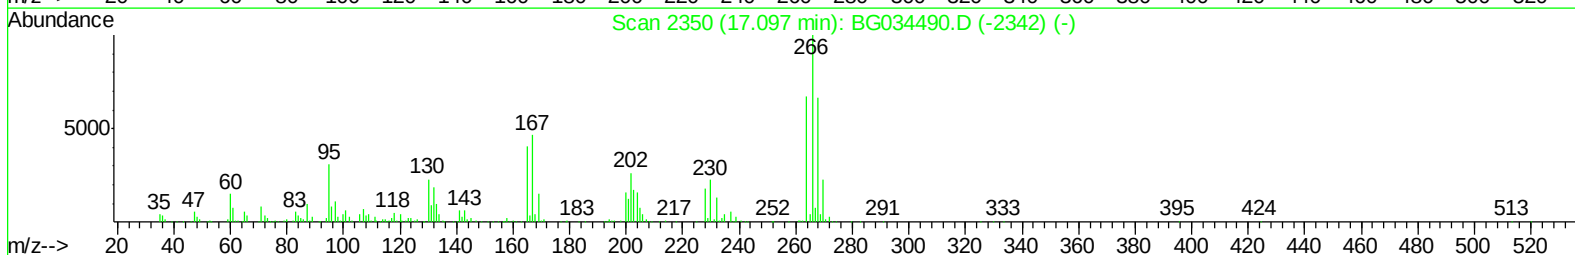
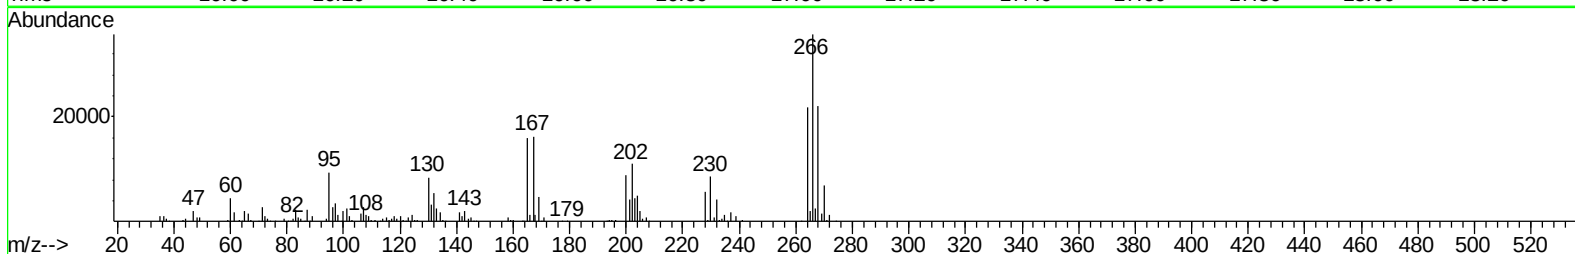


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060718\  
Data File : BG034943.D  
Acq On : 7 Jun 2018 8:03  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 13:02:29 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 05 15:48:31 2018  
Response via : Initial Calibration

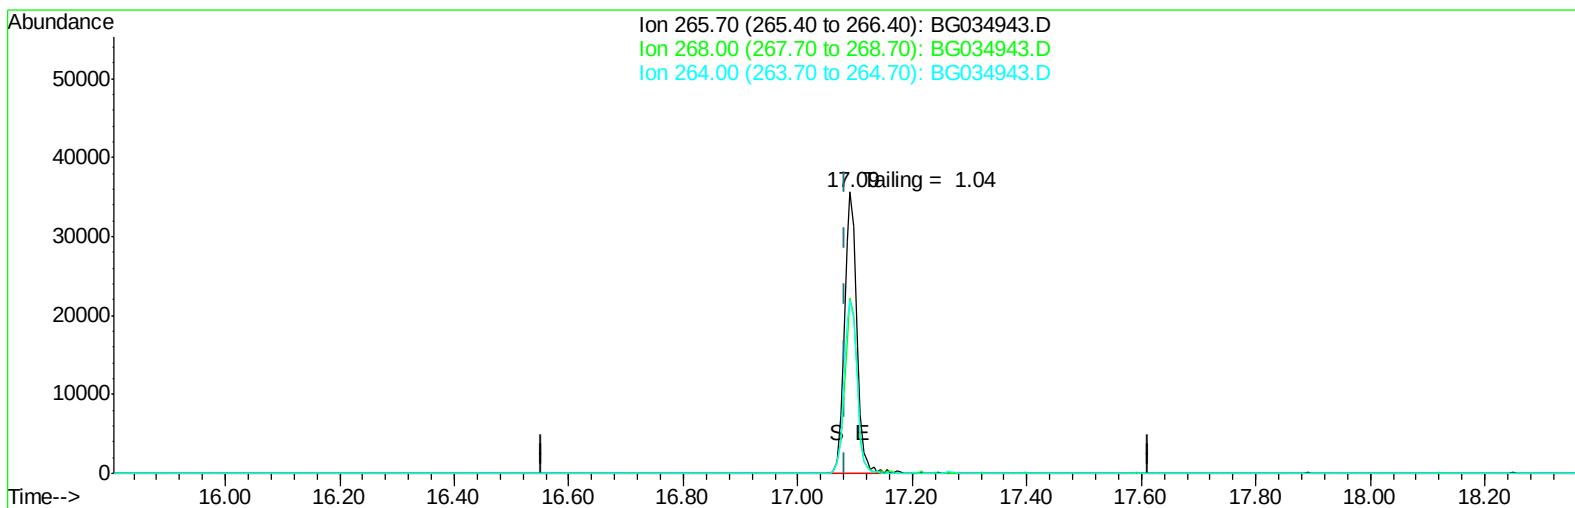

TIC: BG034943.D

(69) Pentachlorophenol (C)




17.092min (+0.009) 30213.97ng

response 52996

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.13 |
| 264.00 | 62.00 | 61.43 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060718\  
 Data File : BG034943.D  
 Acq On : 7 Jun 2018 8:03  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 07 13:02:29 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051618.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 05 15:48:31 2018  
 Response via : Initial Calibration

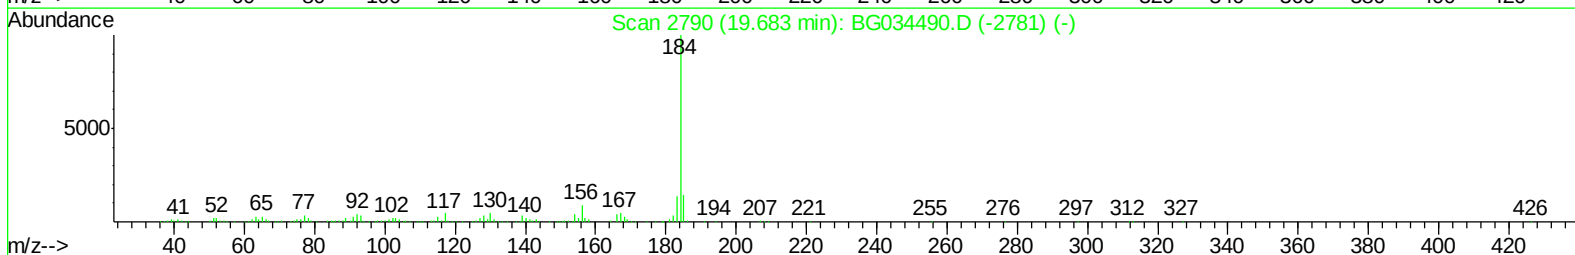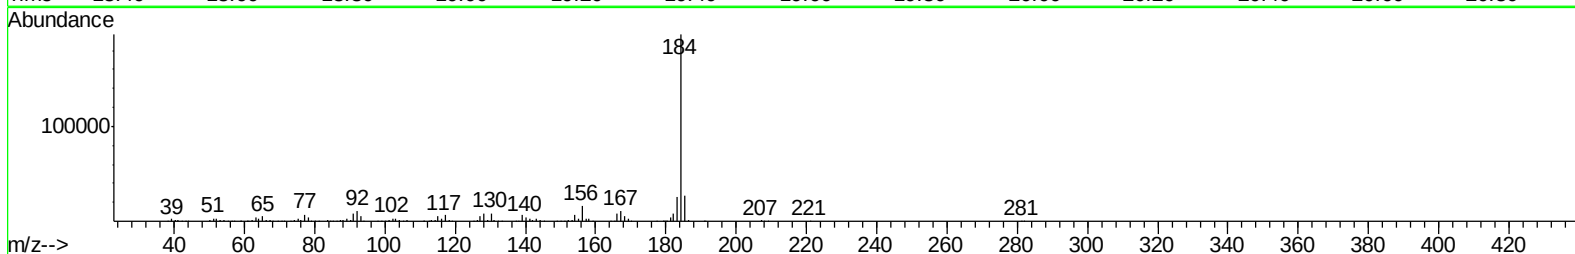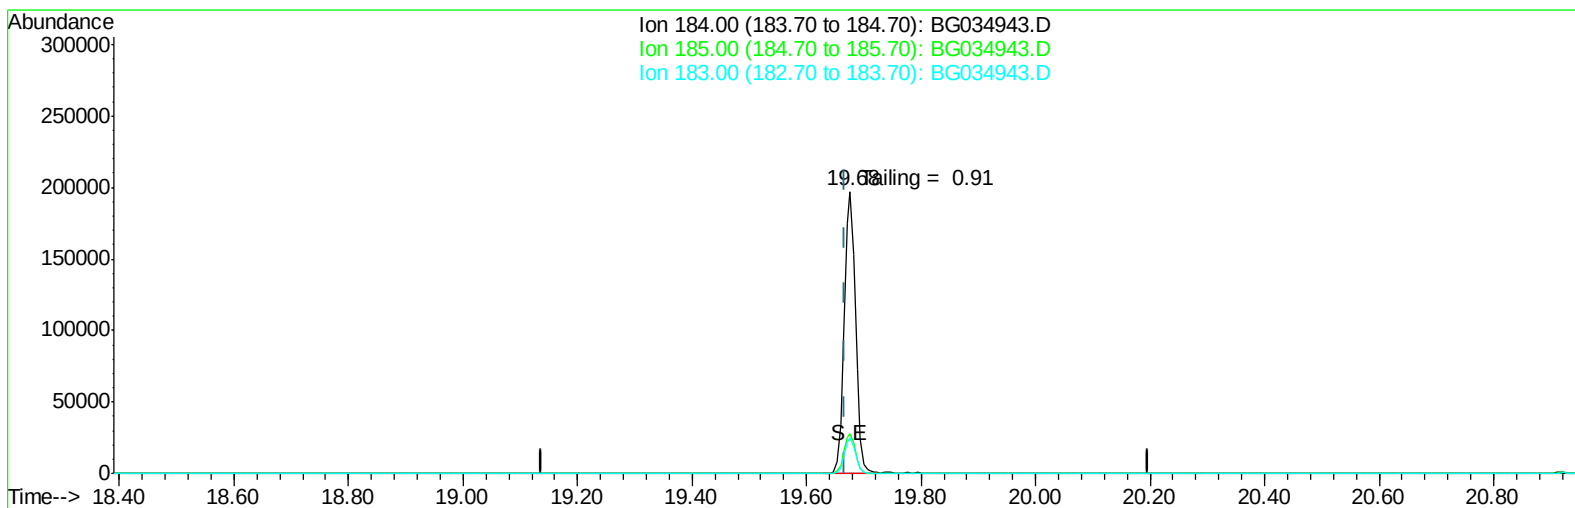

TIC: BG034943.D

(76) Benzidine

19.677min (+0.008) 0.00ng

response 271694

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 13.97 |
| 183.00 | 13.30 | 12.82 |
| 0.00   | 0.00  | 0.00  |