

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060718\
 Data File : BG034980.D
 Acq On : 8 Jun 2018 9:44
 Operator : SJ/JU
 Sample : J3344-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HS-HOUSE-WALL

Quant Time: Jun 08 12:33:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 07 13:13:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	40632	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	140579	20.00	ng	-0.01
38) Acenaphthene-d10	14.70	164	97528	20.00	ng	-0.01
63) Phenanthrene-d10	17.44	188	273884	20.00	ng	-0.01
75) Chrysene-d12	21.71	240	295731	20.00	ng	-0.02
86) Perylene-d12	24.95	264	290197	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	323607	134.41	ng	0.00
7) Phenol-d6	7.23	99	431009	121.29	ng	0.00
23) Nitrobenzene-d5	9.24	82	336850	113.90	ng	-0.01
41) 2,4,6-Tribromophenol	16.18	330	221490	177.41	ng	-0.01
44) 2-Fluorobiphenyl	13.33	172	747909	99.69	ng	-0.01
78) Terphenyl-d14	20.05	244	1465521	103.80	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060718\
Data File : BG034980.D
Acq On : 8 Jun 2018 9:44
Operator : SJ/JU
Sample : J3344-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HS-HOUSE-WALL

Quant Time: Jun 08 12:33:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 07 13:13:20 2018
Response via : Initial Calibration

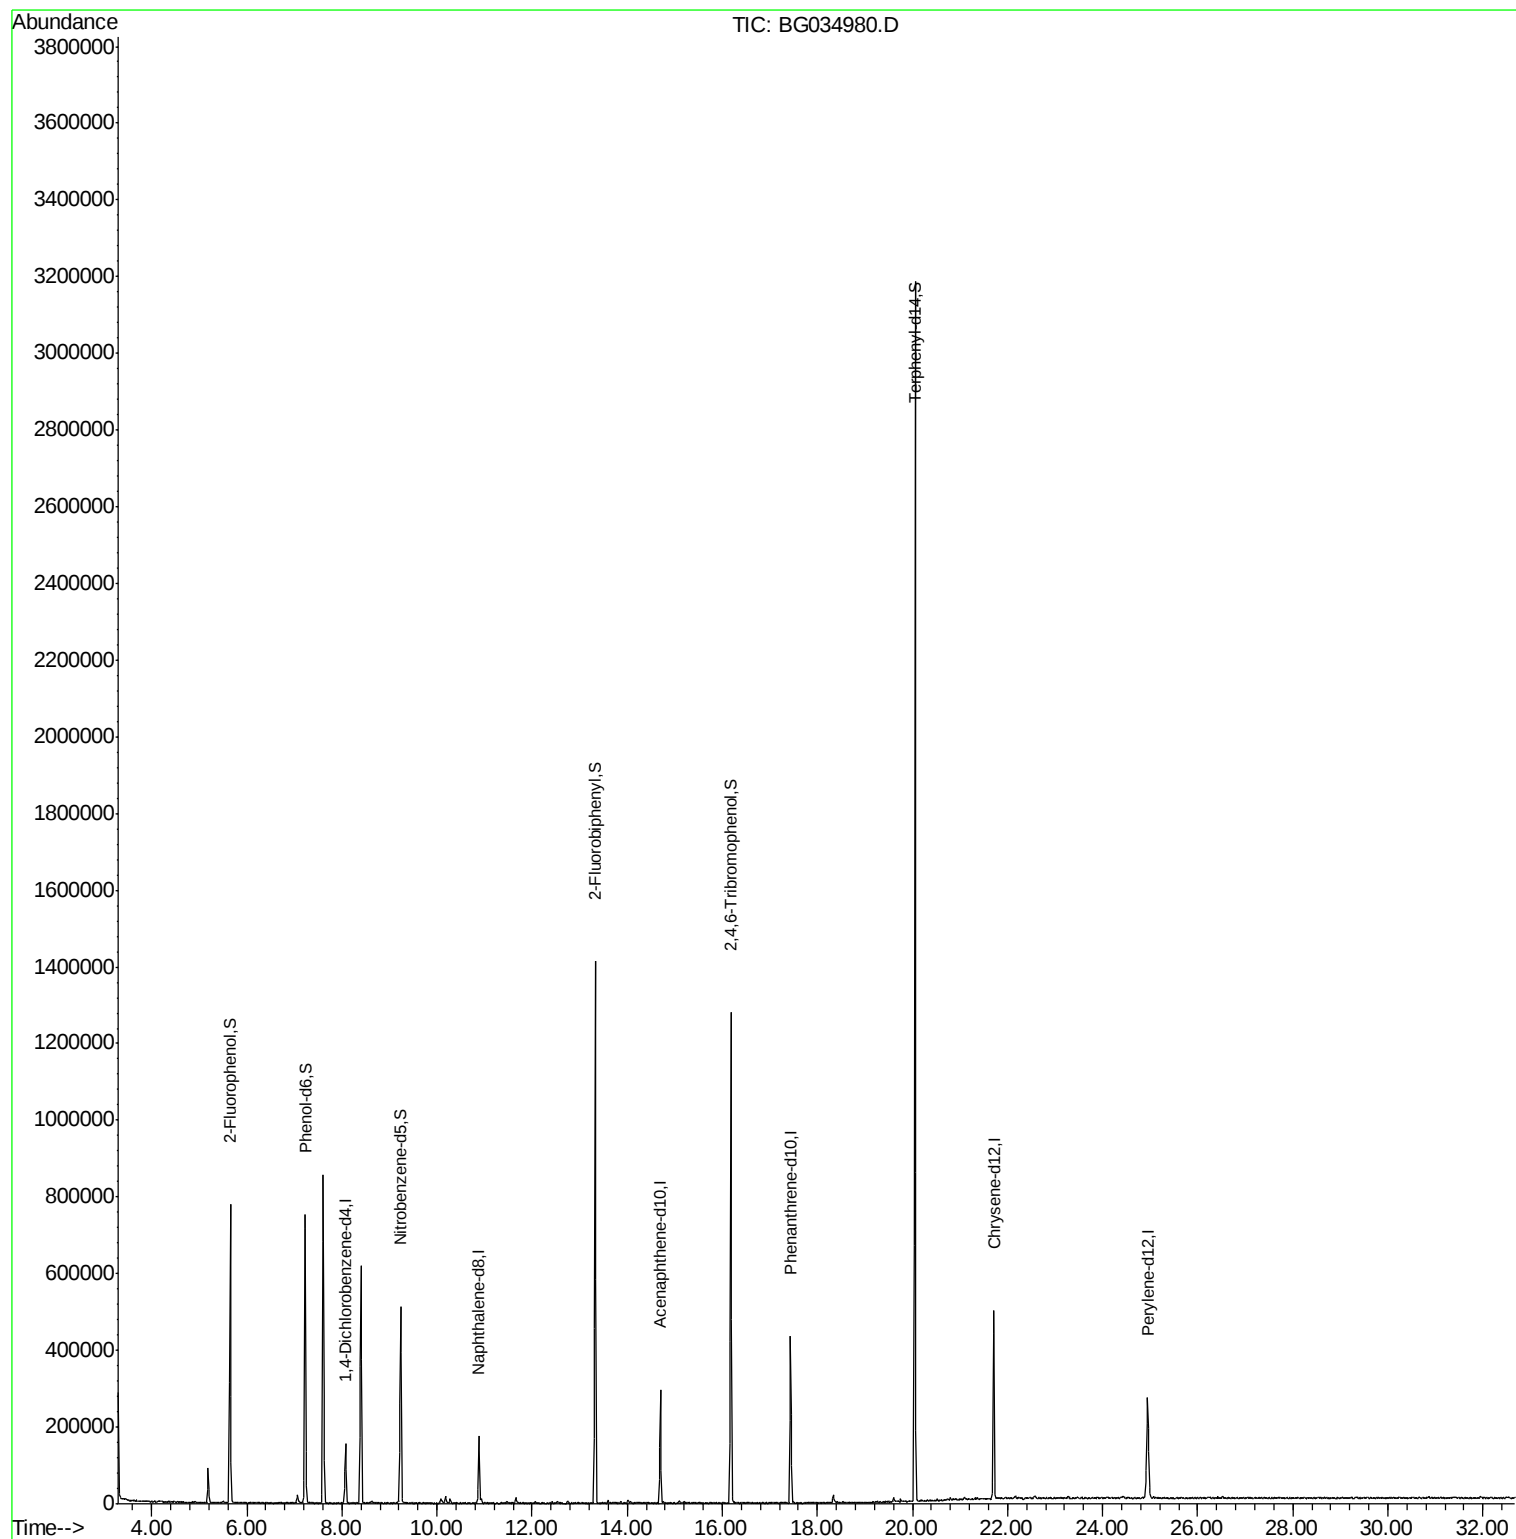

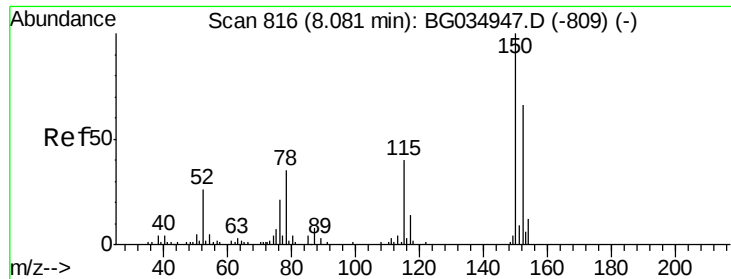


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.08 min Scan# 816
Delta R.T. -0.00 min
Lab File: BG034980.D
Acq: 8 Jun 2018 9:44

Instrument :
BNA_G
ClientSampleId :
HS-HOUSE-WALL

Tot Ion:152 Resp: 40632
Ion Ratio Lower Upper
152 100
150 130.2 126.6 189.8
115 58.7 53.0 79.4

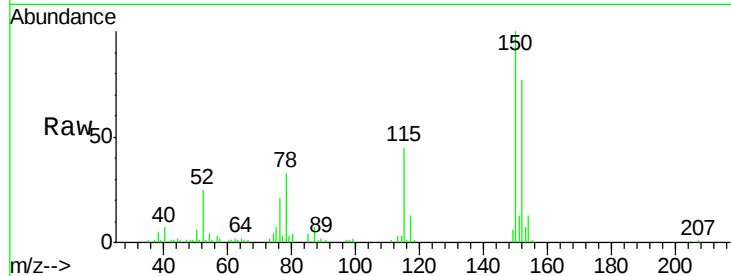


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

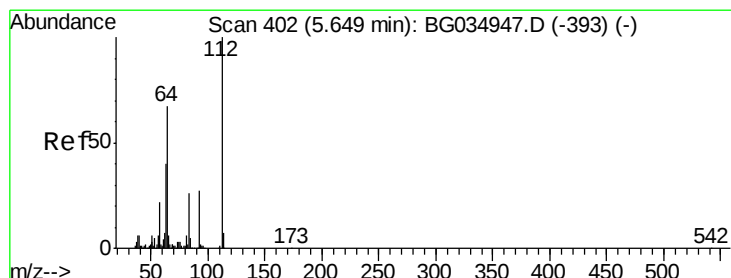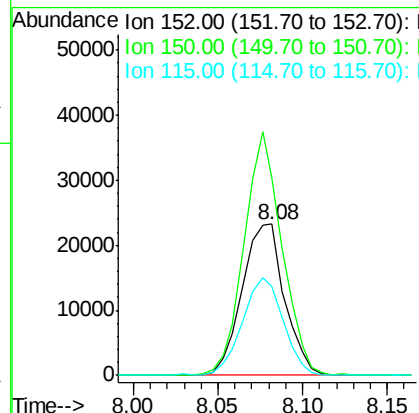



#5


2-Fluorophenol
Concen: 134.407 ng
RT: 5.65 min Scan# 402
Delta R.T. 0.00 min
Lab File: BG034980.D
Acq: 8 Jun 2018 9:44

Tgt Ion:112 Resp: 323607
Ion Ratio Lower Upper
112 100
64 64.5 56.3 84.5
63 35.6 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

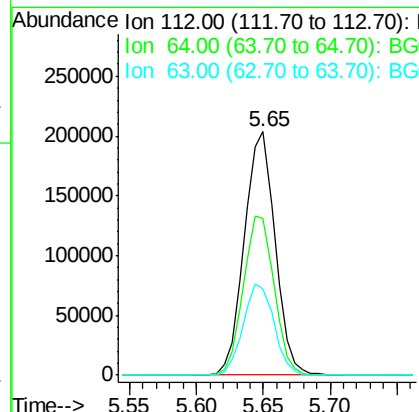

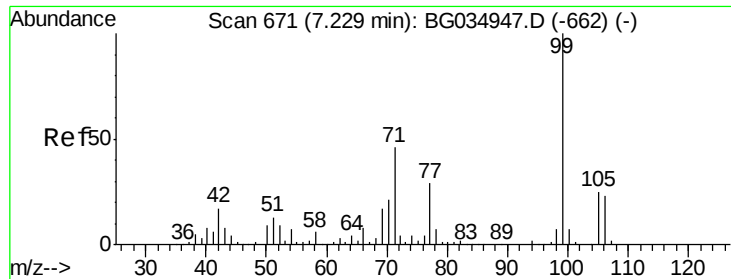

#7

Phenol-d6

Concen: 121.289 ng

RT: 7.23 min Scan# 671

Delta R.T. -0.00 min

Lab File: BG034980.D

Acq: 8 Jun 2018 9:44

Instrument :

BNA_G

ClientSampleId :

HS-HOUSE-WALL


Tot Ion: 99 Resp: 431009

Ion Ratio Lower Upper




99 100

42 16.2 14.1 21.1

71 44.1 26.1 39.1#

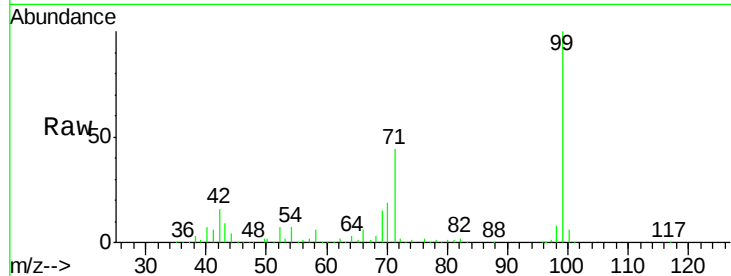

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

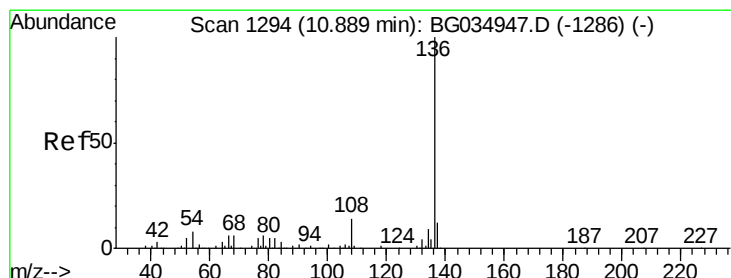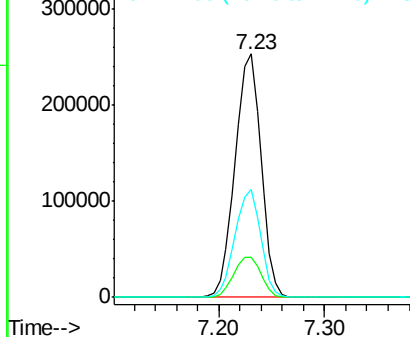

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.88 min Scan# 1293

Delta R.T. -0.01 min

Lab File: BG034980.D

Acq: 8 Jun 2018 9:44

Tgt Ion: 136 Resp: 140579


Ion Ratio Lower Upper

136 100



137 11.0 9.2 13.8


54 6.5 10.3 15.5#

68 5.6 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




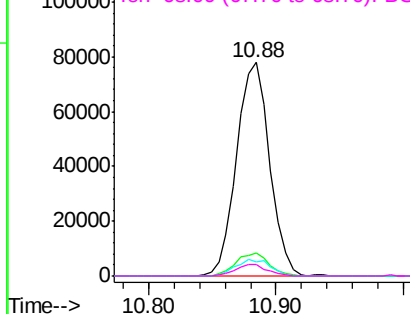




#23
Nitrobenzene-d5
Concen: 113.900 ng
RT: 9.24 min Scan# 1013
Delta R.T. -0.01 min
Lab File: BG034980.D
Acq: 8 Jun 2018 9:44




Instrument :
BNA_G
ClientSampleId :
HS-HOUSE-WALL


Tot Ion	Ratio	Lower	Upper
82	100		
128	32.0	29.7	44.5
54	44.7	43.1	64.7

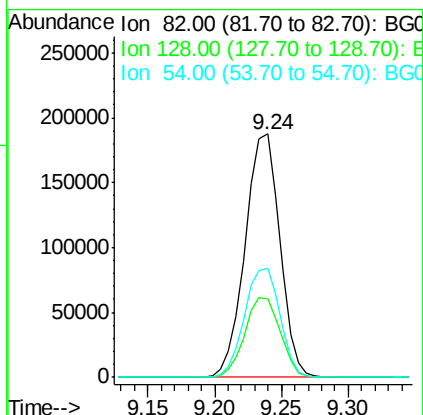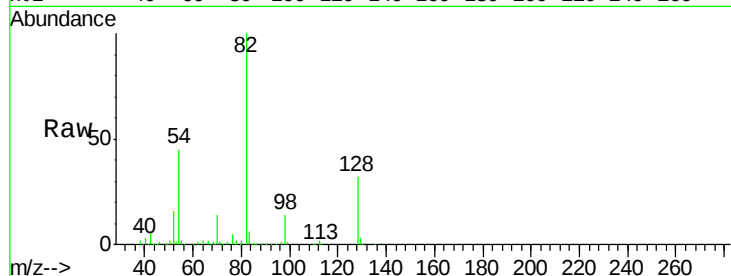

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.70 min Scan# 1942
Delta R.T. -0.01 min
Lab File: BG034980.D
Acq: 8 Jun 2018 9:44

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.4	78.8	118.2
160	46.8	35.4	53.0

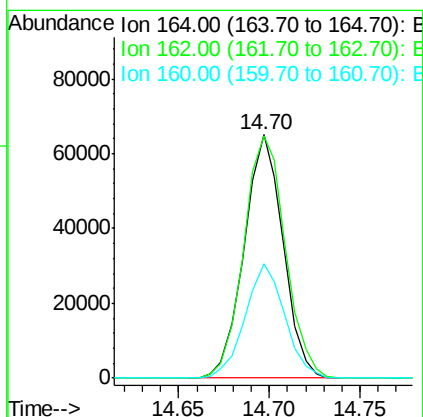


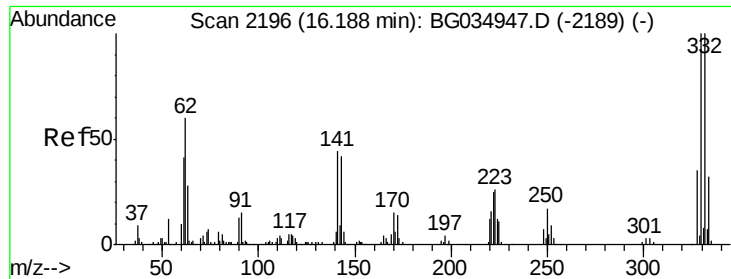




#41
 2,4,6-Tribromophenol
 Concen: 177.407 ng
 RT: 16.18 min Scan# 2195
 Delta R.T. -0.01 min
 Lab File: BG034980.D
 Acq: 8 Jun 2018 9:44

Instrument :
 BNA_G
 ClientSampleId :
 HS-HOUSE-WALL

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.3	77.0	115.6
141	41.9	25.2	37.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

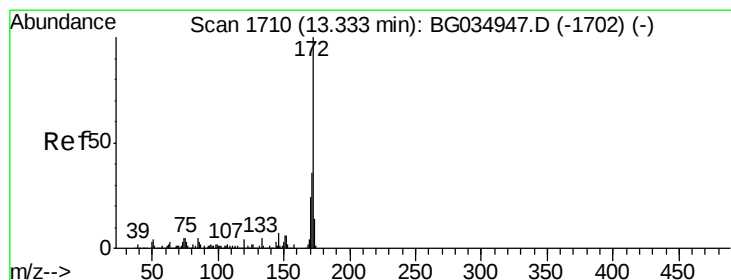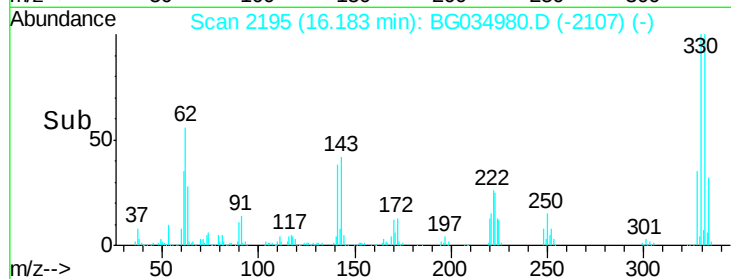
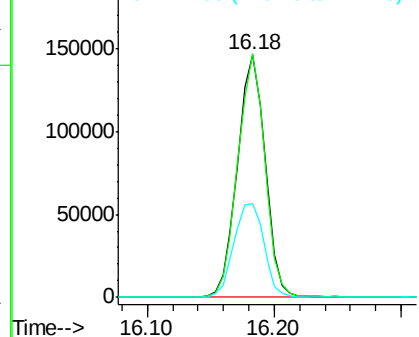



#44
 2-Fluorobiphenyl
 Concen: 99.692 ng
 RT: 13.33 min Scan# 1709
 Delta R.T. -0.01 min
 Lab File: BG034980.D
 Acq: 8 Jun 2018 9:44

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.3	30.0	45.0
170	23.5	19.5	29.3

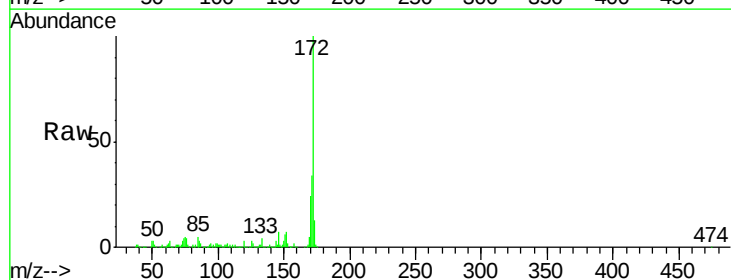

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

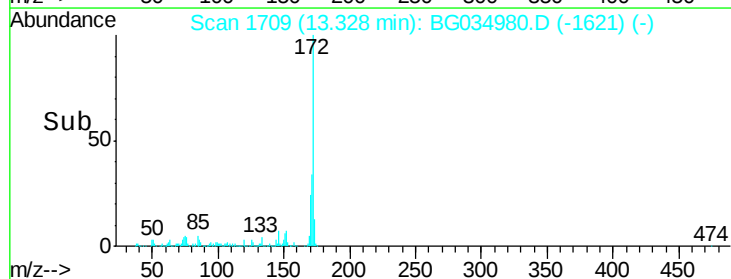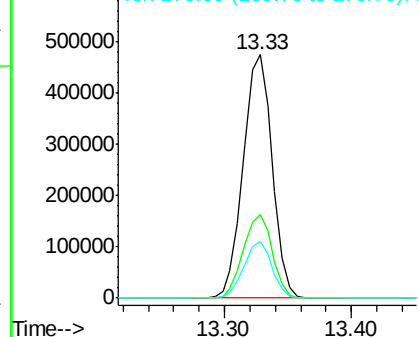



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.44 min Scan# 2409

Delta R.T. -0.01 min

Lab File: BG034980.D

Acq: 8 Jun 2018 9:44

Instrument :

BNA_G

ClientSampleId :

HS-HOUSE-WALL


Tot Ion:188 Resp: 273884

Ion Ratio Lower Upper

188 100

94 5.8 6.9 10.3#




80 8.0 7.7 11.5

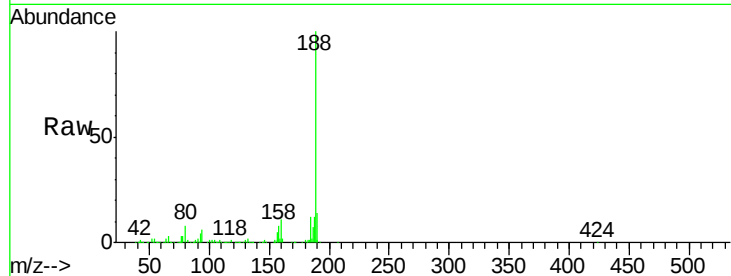

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

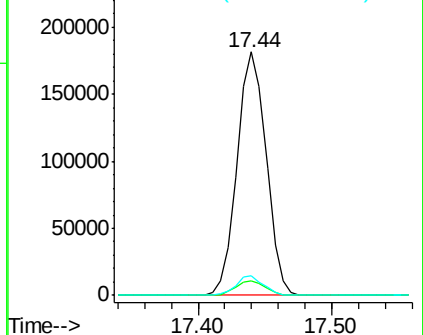

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.71 min Scan# 3136

Delta R.T. -0.02 min

Lab File: BG034980.D

Acq: 8 Jun 2018 9:44


Tgt Ion:240 Resp: 295731

Ion Ratio Lower Upper

240 100

120 6.1 6.8 10.2#



236 26.6 20.9 31.3




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

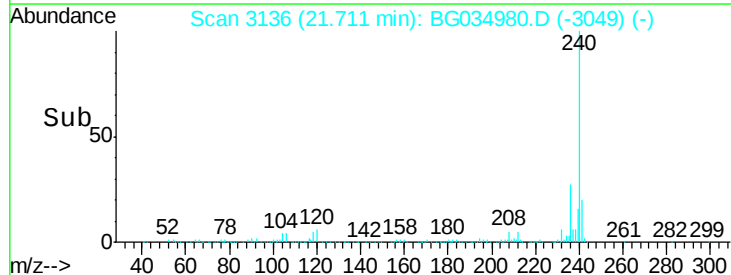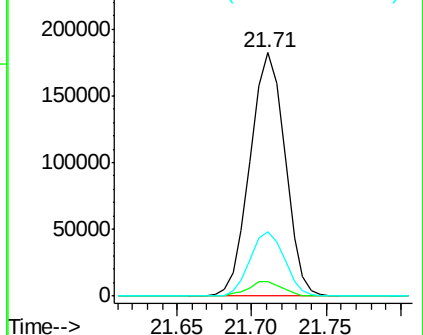

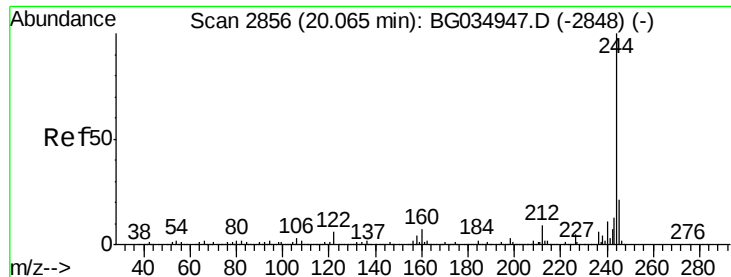

#78

Terphenyl-d14

Concen: 103.803 ng

RT: 20.05 min Scan# 2854

Delta R.T. -0.01 min

Lab File: BG034980.D

Acq: 8 Jun 2018 9:44

Instrument :

BNA_G

ClientSampleId :

HS-HOUSE-WALL


Tot Ion:244 Resp: 1465521

Ion Ratio Lower Upper

244 100

212 9.6 5.8 8.8#




122 7.1 7.0 10.4

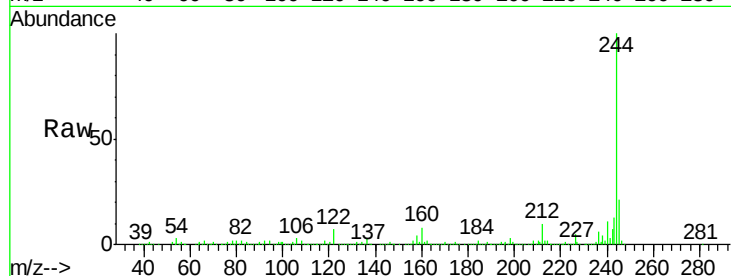

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

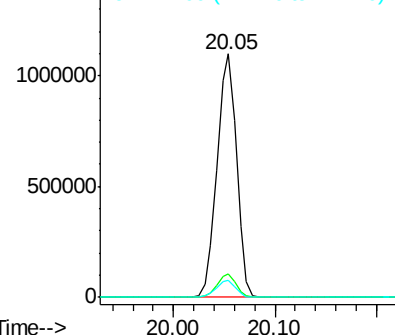

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.95 min Scan# 3688

Delta R.T. -0.03 min

Lab File: BG034980.D

Acq: 8 Jun 2018 9:44


Tgt Ion:264 Resp: 290197

Ion Ratio Lower Upper

264 100

260 20.4 17.4 26.0

265 22.3 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

