


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060718\
 Data File : BG034943.D
 Acq On : 7 Jun 2018 8:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 07 13:13:20 2018

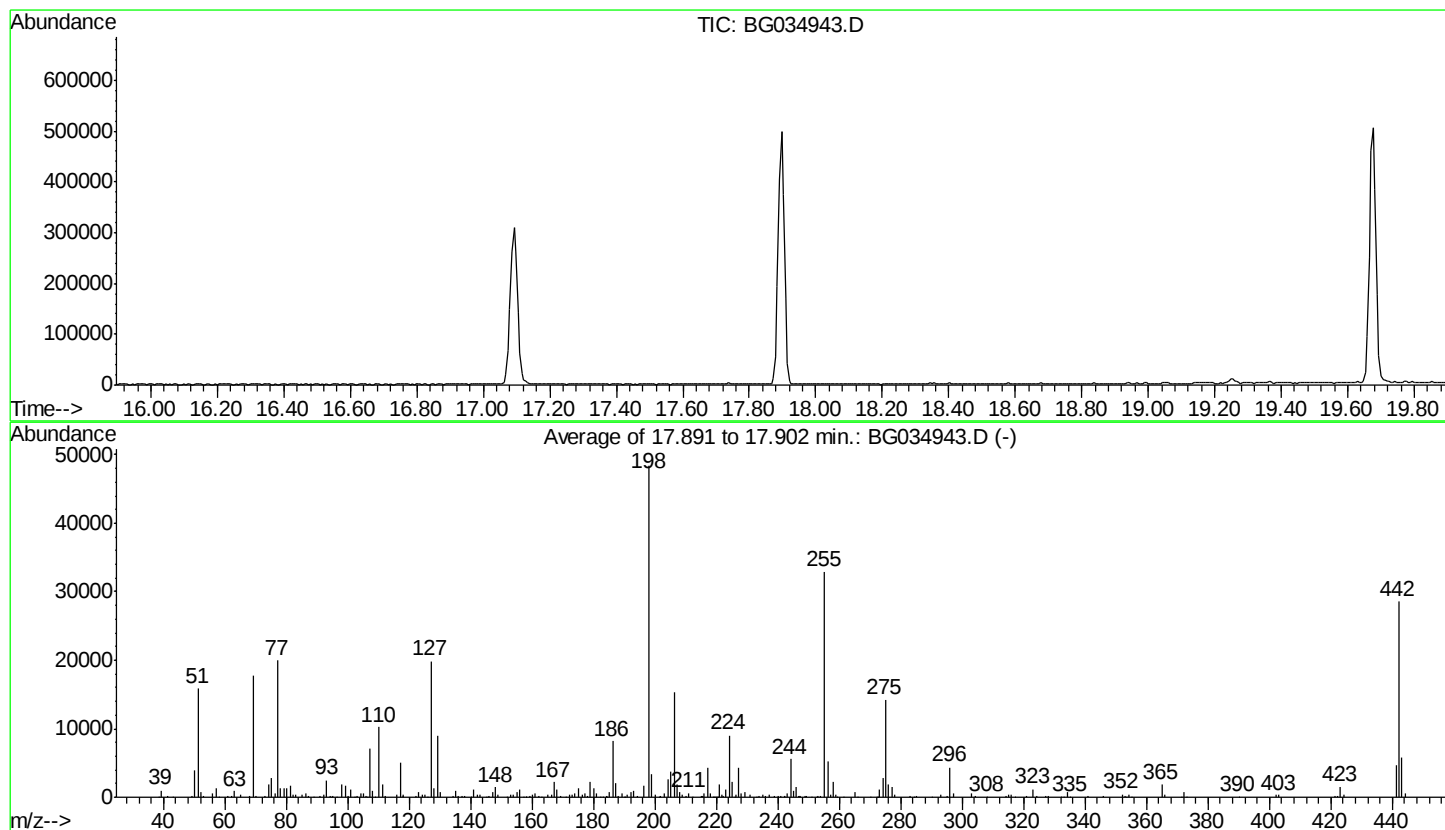

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	15802	PASS
68	69	0.00	2	1.6	277	PASS
69	198	0.00	100	36.6	17738	PASS
70	69	0.00	2	0.6	106	PASS
127	198	10	80	41.1	19893	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48402	PASS
199	198	5	9	7.1	3432	PASS
275	198	10	60	29.3	14202	PASS
365	198	1	100	3.8	1857	PASS
441	443	0.01	100	80.3	4661	PASS
442	198	50	100	59.0	28549	PASS
443	442	15	24	20.3	5803	PASS