


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060718\
 Data File : BG034952.D
 Acq On : 7 Jun 2018 14:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 07 13:13:20 2018

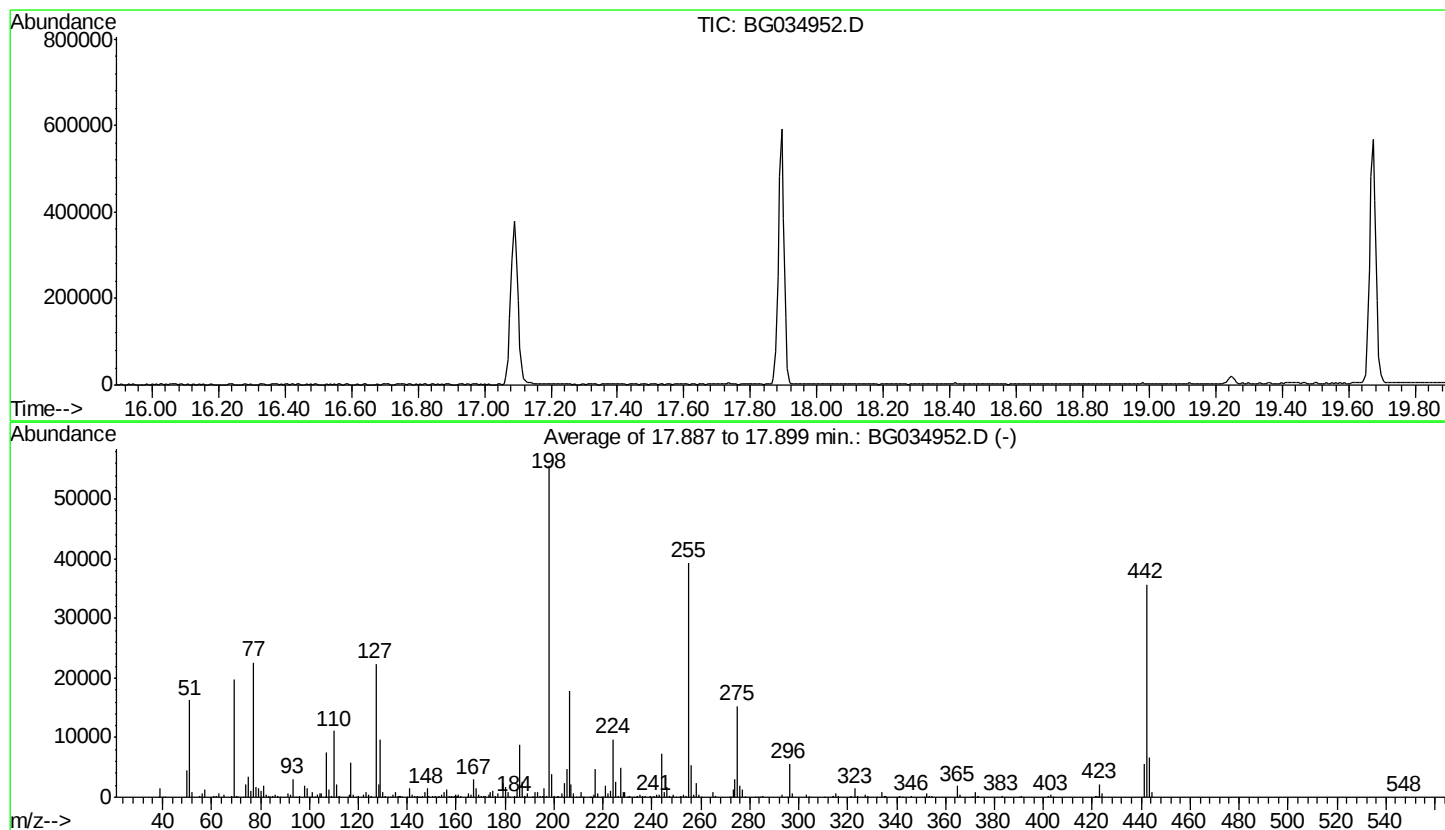

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	16286	PASS
68	69	0.00	2	0.6	119	PASS
69	198	0.00	100	35.7	19866	PASS
70	69	0.00	2	0.6	118	PASS
127	198	10	80	40.2	22388	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55624	PASS
199	198	5	9	6.9	3844	PASS
275	198	10	60	27.5	15313	PASS
365	198	1	100	3.4	1916	PASS
441	443	0.01	100	83.0	5529	PASS
442	198	50	100	64.1	35680	PASS
443	442	15	24	18.7	6658	PASS