


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060718\
 Data File : BG034971.D
 Acq On : 8 Jun 2018 3:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 07 13:13:20 2018

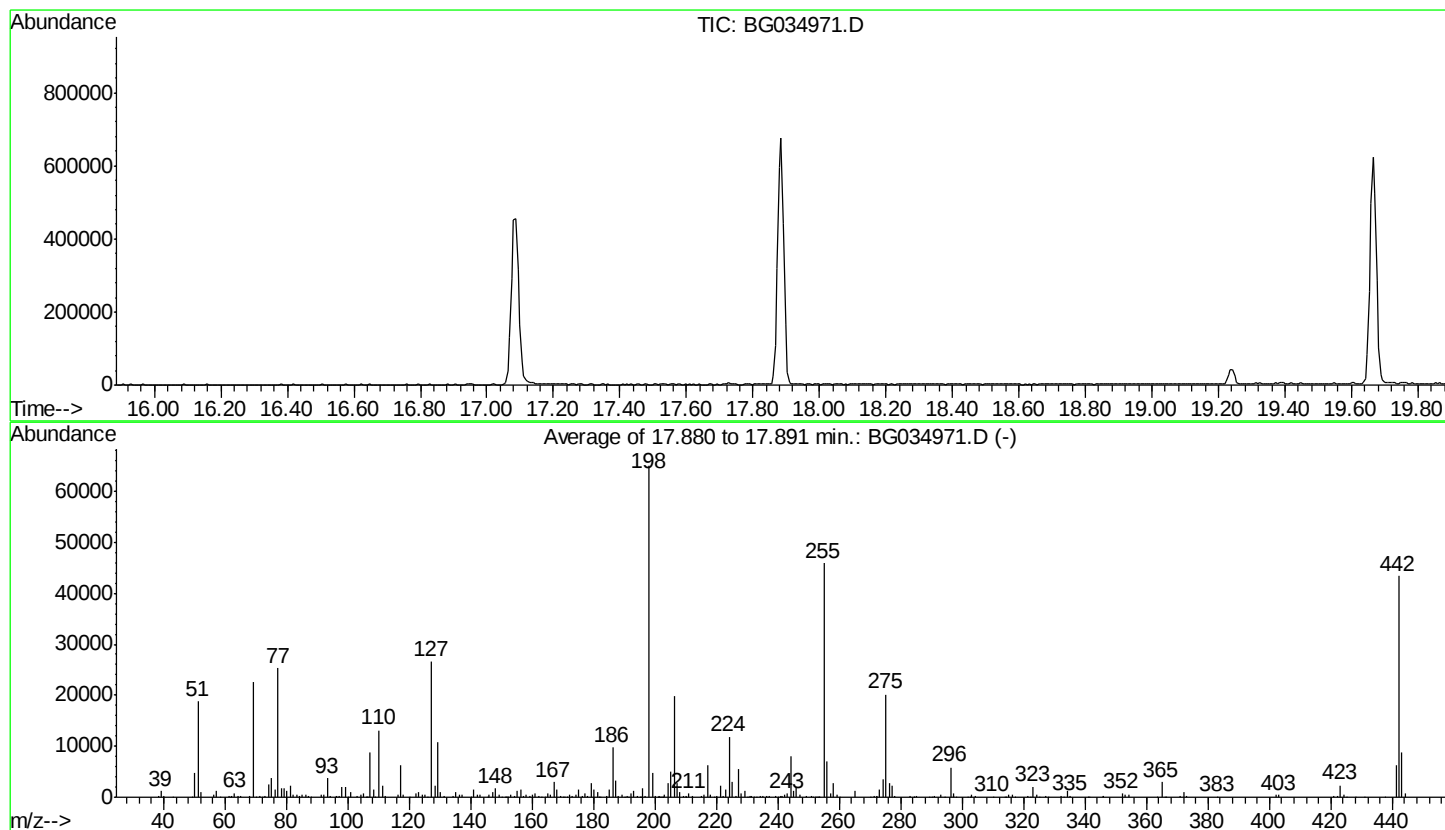

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	18736	PASS
68	69	0.00	2	1.5	332	PASS
69	198	0.00	100	34.9	22716	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	40.8	26522	PASS
197	198	0.00	2	0.3	191	PASS
198	198	100	100	100.0	65029	PASS
199	198	5	9	7.4	4819	PASS
275	198	10	60	30.9	20093	PASS
365	198	1	100	4.5	2913	PASS
441	443	0.01	100	73.2	6388	PASS
442	198	50	100	66.7	43362	PASS
443	442	15	24	20.1	8727	PASS