

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060719\
 Data File : BG041117.D
 Acq On : 8 Jun 2019 3:29
 Operator : HP/JU
 Sample : PB120423BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120423BL

Quant Time: Jun 08 18:14:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 08 17:33:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	41169	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	170921	20.00	ng	0.00
39) Acenaphthene-d10	14.73	164	136489	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	350075	20.00	ng	0.00
76) Chrysene-d12	21.76	240	352458	20.00	ng	0.00
87) Perylene-d12	25.08	264	362504	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	316174	138.48	ng	0.00
7) Phenol-d6	7.25	99	468691	132.92	ng	0.00
23) Nitrobenzene-d5	9.28	82	312276	81.11	ng	0.00
42) 2,4,6-Tribromophenol	16.23	330	254096	125.40	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	806093	85.05	ng	0.00
79) Terphenyl-d14	20.07	244	1453704	87.54	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060719\
Data File : BG041117.D
Acq On : 8 Jun 2019 3:29
Operator : HP/JU
Sample : PB120423BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120423BL

Quant Time: Jun 08 18:14:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 08 17:33:39 2019
Response via : Initial Calibration

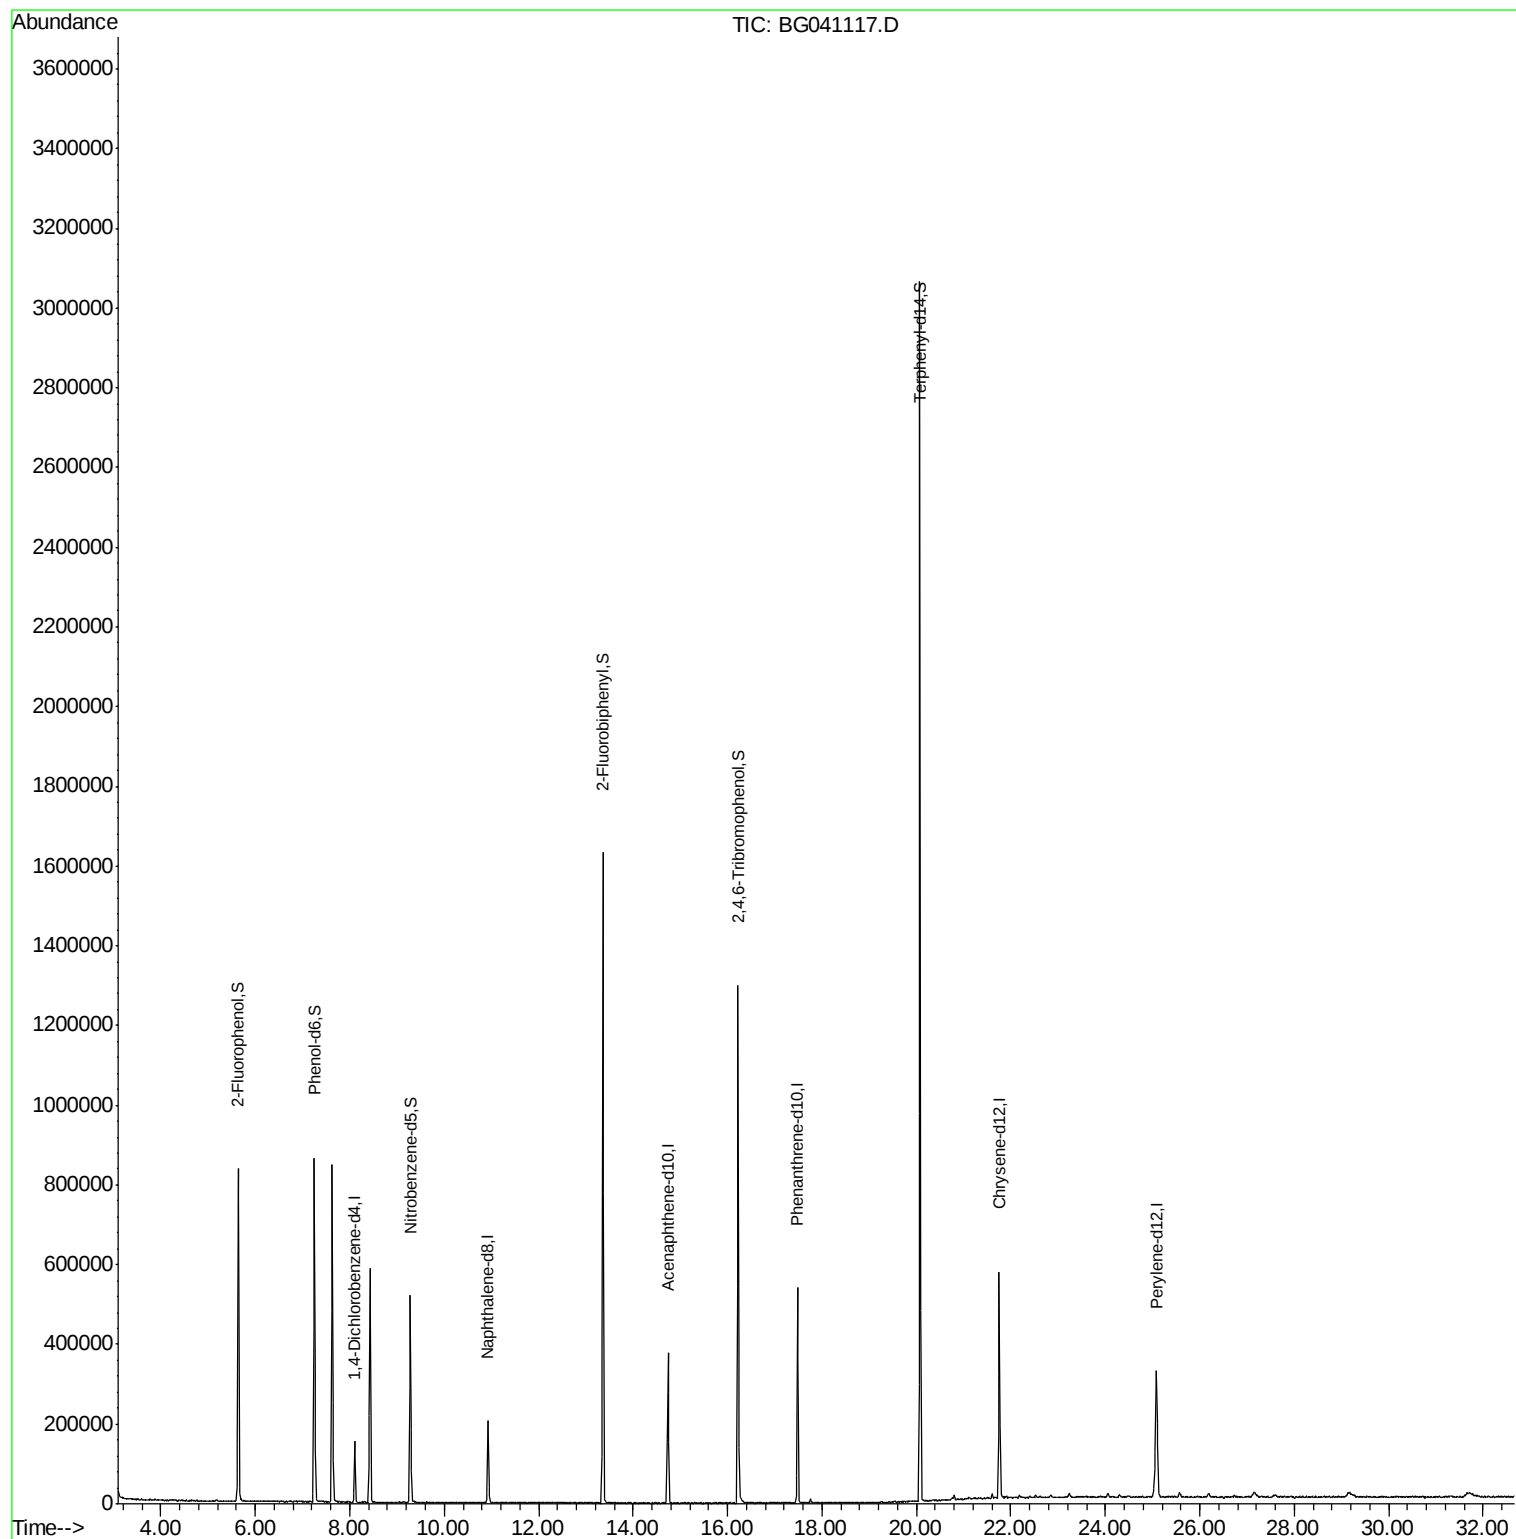




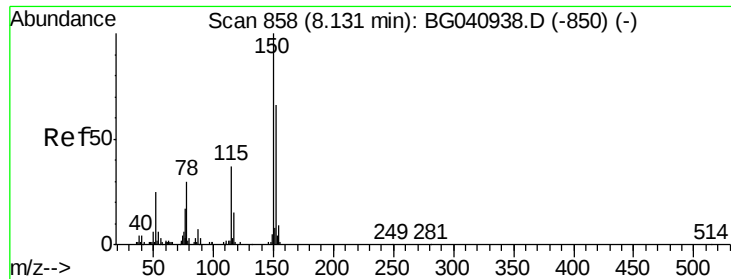


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.11 min Scan# 854
Delta R.T. 0.00 min
Lab File: BG041117.D
Acq: 8 Jun 2019 3:29

Instrument :
BNA_G
ClientSampleId :
PB120423BL




Tot Ion:152 Resp: 41169
Ion Ratio Lower Upper
152 100
150 166.6 111.7 167.5
115 58.6 48.6 73.0

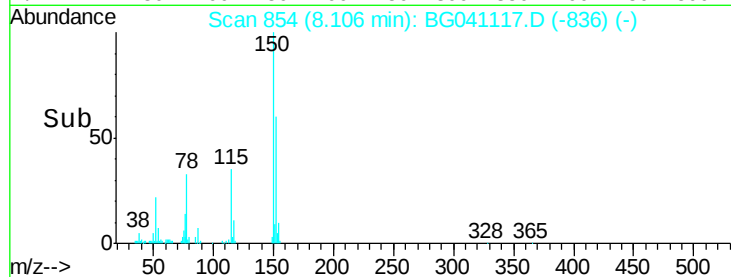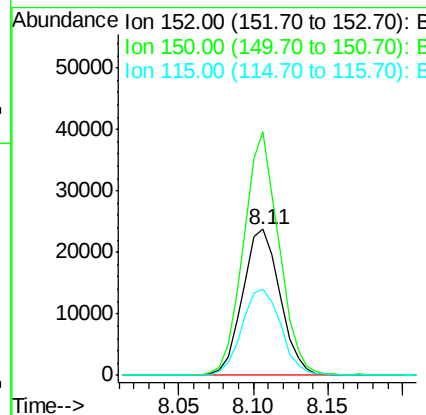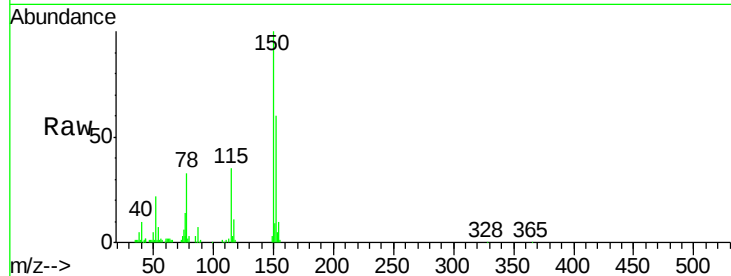


#5

2-Fluorophenol
Concen: 138.485 ng
RT: 5.64 min Scan# 434
Delta R.T. -0.00 min
Lab File: BG041117.D
Acq: 8 Jun 2019 3:29

Tgt Ion:112 Resp: 316174
Ion Ratio Lower Upper
112 100
64 71.1 54.5 81.7
63 42.2 32.2 48.2

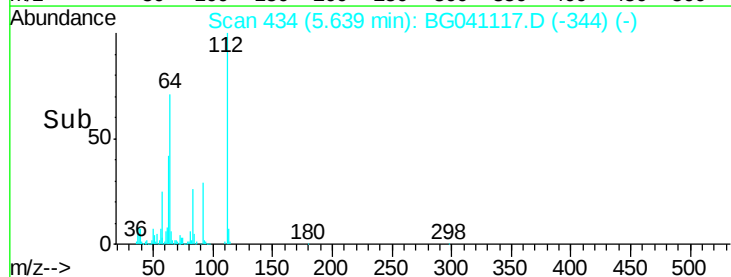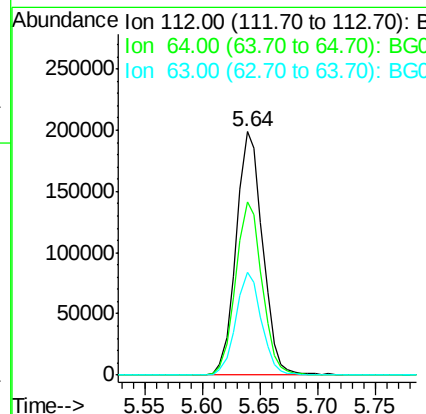

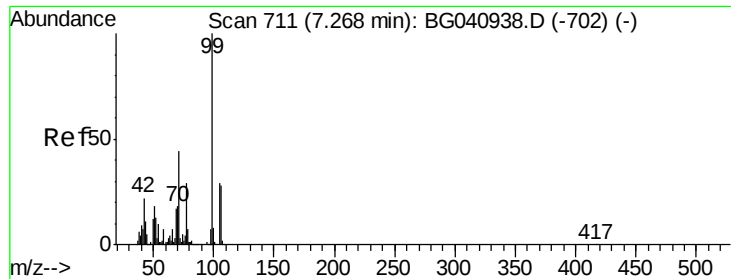

#7

Phenol-d6

Concen: 132.924 ng

RT: 7.25 min Scan# 709

Delta R.T. 0.00 min

Lab File: BG041117.D

Acq: 8 Jun 2019 3:29

Instrument :

BNA_G

ClientSampleId :

PB120423BL


Tot Ion: 99 Resp: 468691

Ion Ratio Lower Upper




99 100

42 22.5 18.8 28.2

71 43.7 35.6 53.4

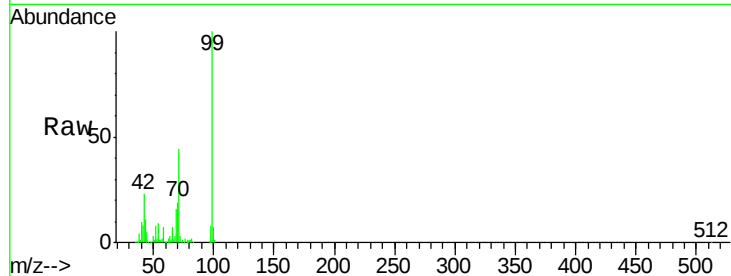

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

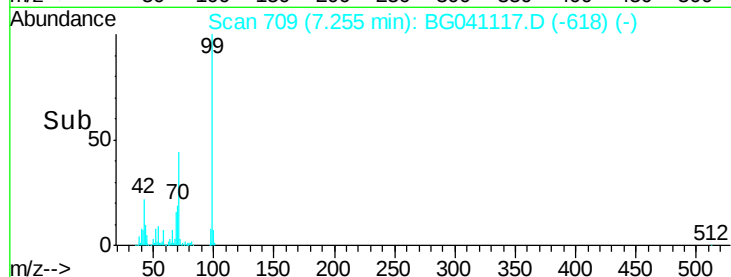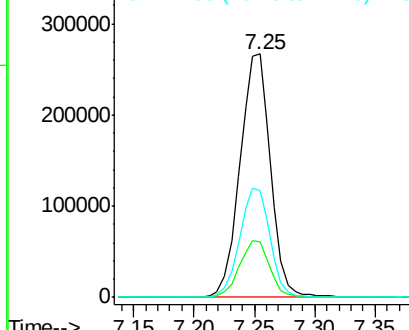

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.93 min Scan# 1334

Delta R.T. -0.00 min

Lab File: BG041117.D

Acq: 8 Jun 2019 3:29

Tgt Ion: 136 Resp: 170921


Ion Ratio Lower Upper

136 100



137 11.9 8.9 13.3

54 7.7 7.4 11.2

68 5.0 4.0 6.0



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



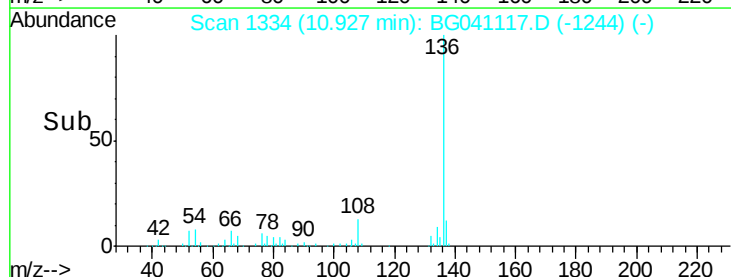
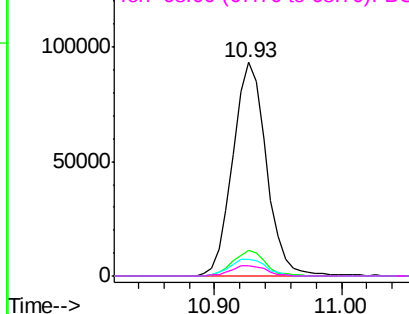




#23
Nitrobenzene-d5
Concen: 81.108 ng
RT: 9.28 min Scan# 1054
Delta R.T. -0.00 min
Lab File: BG041117.D
Acq: 8 Jun 2019 3:29




Instrument :
BNA_G
ClientSampleId :
PB120423BL


Tot Ion: 82 Resp: 312276
Ion Ratio Lower Upper
82 100
128 38.6 29.8 44.6
54 53.0 43.6 65.4

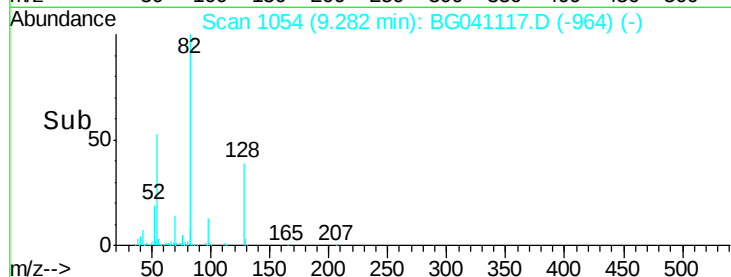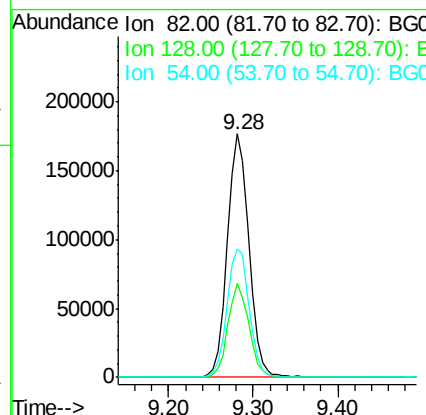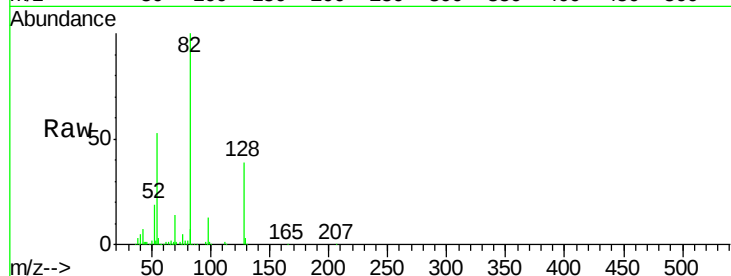

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1982
Delta R.T. -0.01 min
Lab File: BG041117.D
Acq: 8 Jun 2019 3:29

Tgt Ion: 164 Resp: 136489
Ion Ratio Lower Upper
164 100
162 103.2 85.4 128.0
160 45.6 37.1 55.7

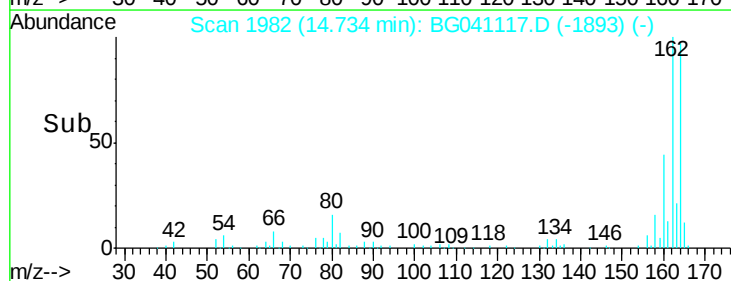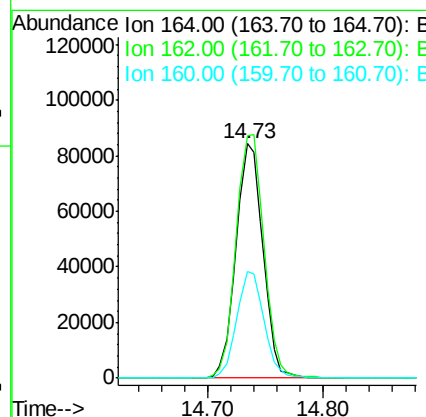

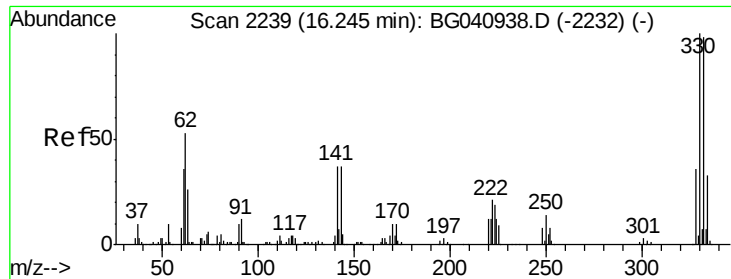

#42

2,4,6-Tribromophenol

Concen: 125.401 ng

RT: 16.23 min Scan# 2236

Delta R.T. 0.00 min

Lab File: BG041117.D

Acq: 8 Jun 2019 3:29

Instrument :

BNA_G

ClientSampleId :

PB120423BL


Tot Ion:330 Resp: 254096

Ion Ratio Lower Upper

330 100

332 96.8 77.9 116.9




141 35.9 29.0 43.4



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

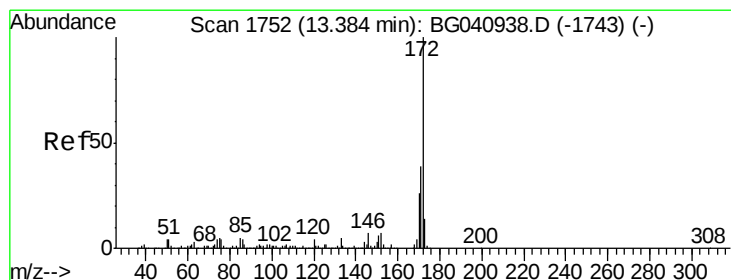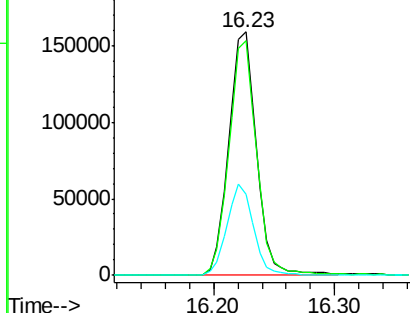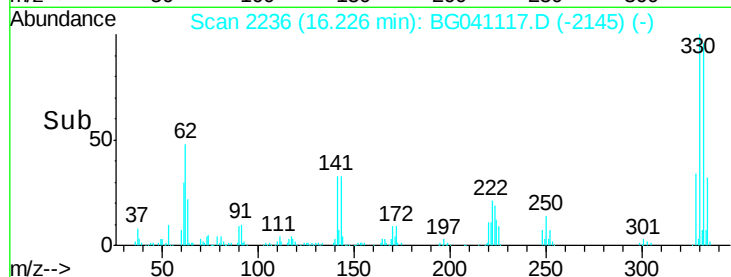

#45

2-Fluorobiphenyl

Concen: 85.052 ng

RT: 13.36 min Scan# 1748

Delta R.T. -0.00 min

Lab File: BG041117.D

Acq: 8 Jun 2019 3:29


Tgt Ion:172 Resp: 806093

Ion Ratio Lower Upper

172 100

171 38.0 30.8 46.2



170 25.4 21.3 31.9

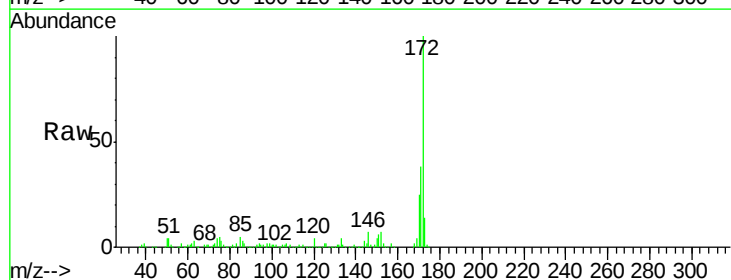


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



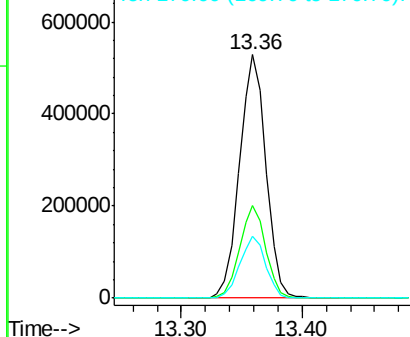
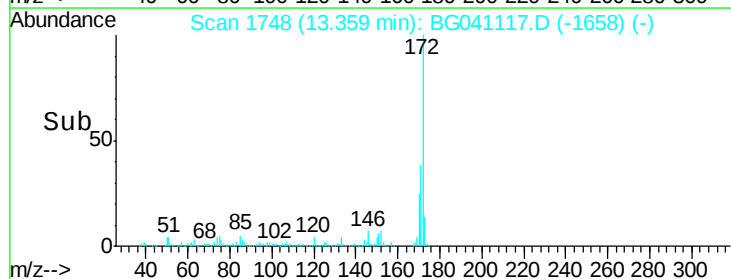


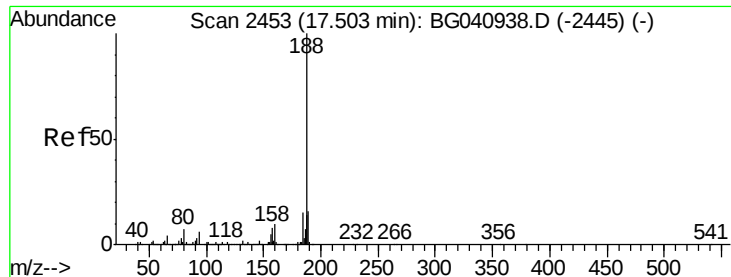

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.48 min Scan# 2449
Delta R.T. -0.00 min
Lab File: BG041117.D
Acq: 8 Jun 2019 3:29




Instrument :
BNA_G
ClientSampleId :
PB120423BL


Tot Ion:188 Resp: 350075
Ion Ratio Lower Upper
188 100
94 5.2 4.6 7.0
80 7.0 5.8 8.8

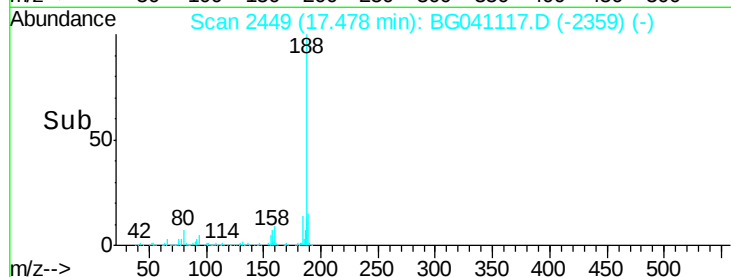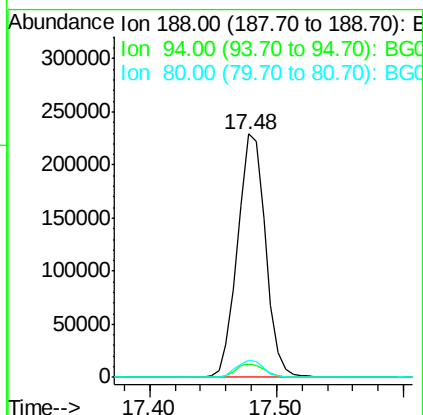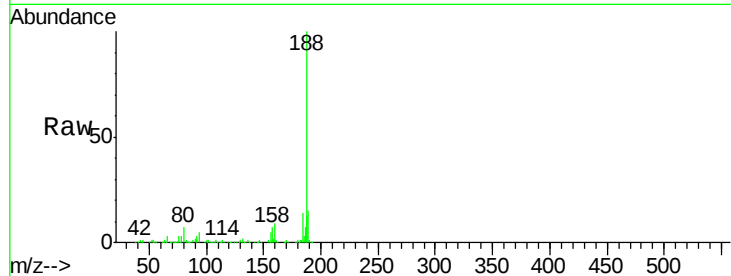

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.76 min Scan# 3177
Delta R.T. -0.01 min
Lab File: BG041117.D
Acq: 8 Jun 2019 3:29

Tgt Ion:240 Resp: 352458
Ion Ratio Lower Upper
240 100
120 5.5 4.6 6.8
236 25.4 20.6 31.0

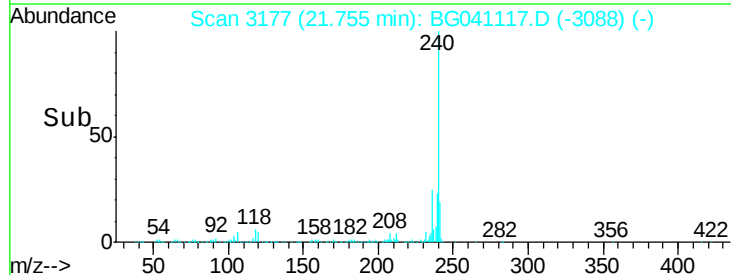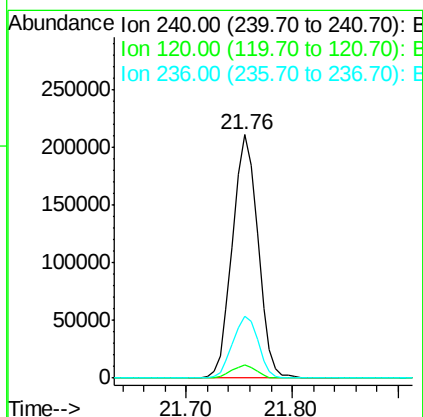

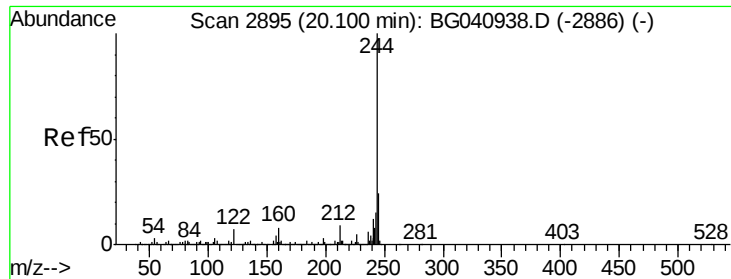

#79

Terphenyl-d14

Concen: 87.536 ng

RT: 20.07 min Scan# 2891

Delta R.T. -0.00 min

Lab File: BG041117.D

Acq: 8 Jun 2019 3:29

Instrument :

BNA_G

ClientSampleId :

PB120423BL


Tot Ion:244 Resp: 1453704

Ion	Ratio	Lower	Upper
244	100		
212	8.5	6.9	10.3
122	7.3	5.4	8.0

244 100

212 8.5 6.9 10.3




122 7.3 5.4 8.0

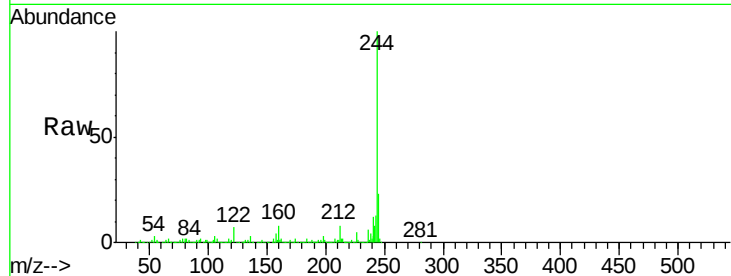

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

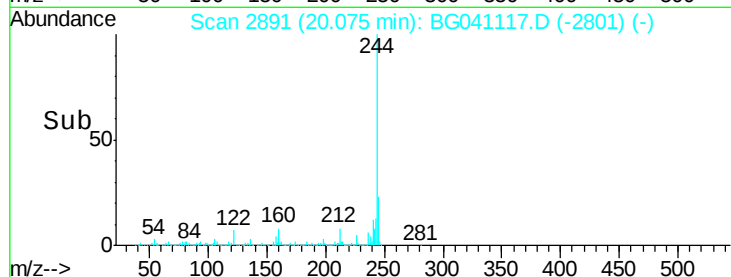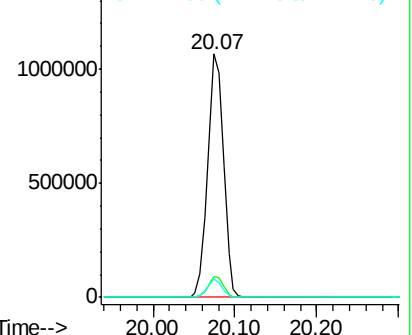

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.08 min Scan# 3743

Delta R.T. -0.00 min

Lab File: BG041117.D

Acq: 8 Jun 2019 3:29


Tgt Ion:264 Resp: 362504

Ion	Ratio	Lower	Upper
264	100		
260	22.7	19.1	28.7
265	21.5	17.6	26.4

264 100

260 22.7 19.1 28.7

265 21.5 17.6 26.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

