

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060719\
 Data File : BG041117.D
 Acq On : 8 Jun 2019 3:29
 Operator : HP/JU
 Sample : PB120423BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120423BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.639	427	434	448	rBV	834745	1314738	32.75%	7.011%
2	7.249	700	708	720	rBV	863405	1529678	38.11%	8.157%
3	7.631	763	773	782	rBV	846645	1435169	35.75%	7.653%
4	8.106	846	854	865	rBV	152940	263023	6.55%	1.403%
5	8.430	901	909	919	rBV	587905	1004466	25.02%	5.356%
6	9.282	1046	1054	1066	rBV	518764	921983	22.97%	4.916%
7	10.927	1326	1334	1346	rBV	207057	380773	9.49%	2.030%
8	13.359	1741	1748	1760	rBV	1632169	2465233	61.41%	13.146%
9	14.740	1975	1983	1999	rVB2	377807	642090	16.00%	3.424%
10	16.220	2228	2235	2253	rBV	1300252	2072492	51.63%	11.051%
11	17.478	2443	2449	2463	rVB2	540875	837081	20.85%	4.464%
12	20.075	2885	2891	2897	rBV	3060435	4014113	100.00%	21.405%
13	21.755	3168	3177	3184	rBV	569058	970176	24.17%	5.173%
14	25.081	3731	3743	3755	rVB2	315339	902336	22.48%	4.812%


Sum of corrected areas: 18753351

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060719\
Data File : BG041117.D
Acq On : 8 Jun 2019 3:29
Operator : HP/JU
Sample : PB120423BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120423BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

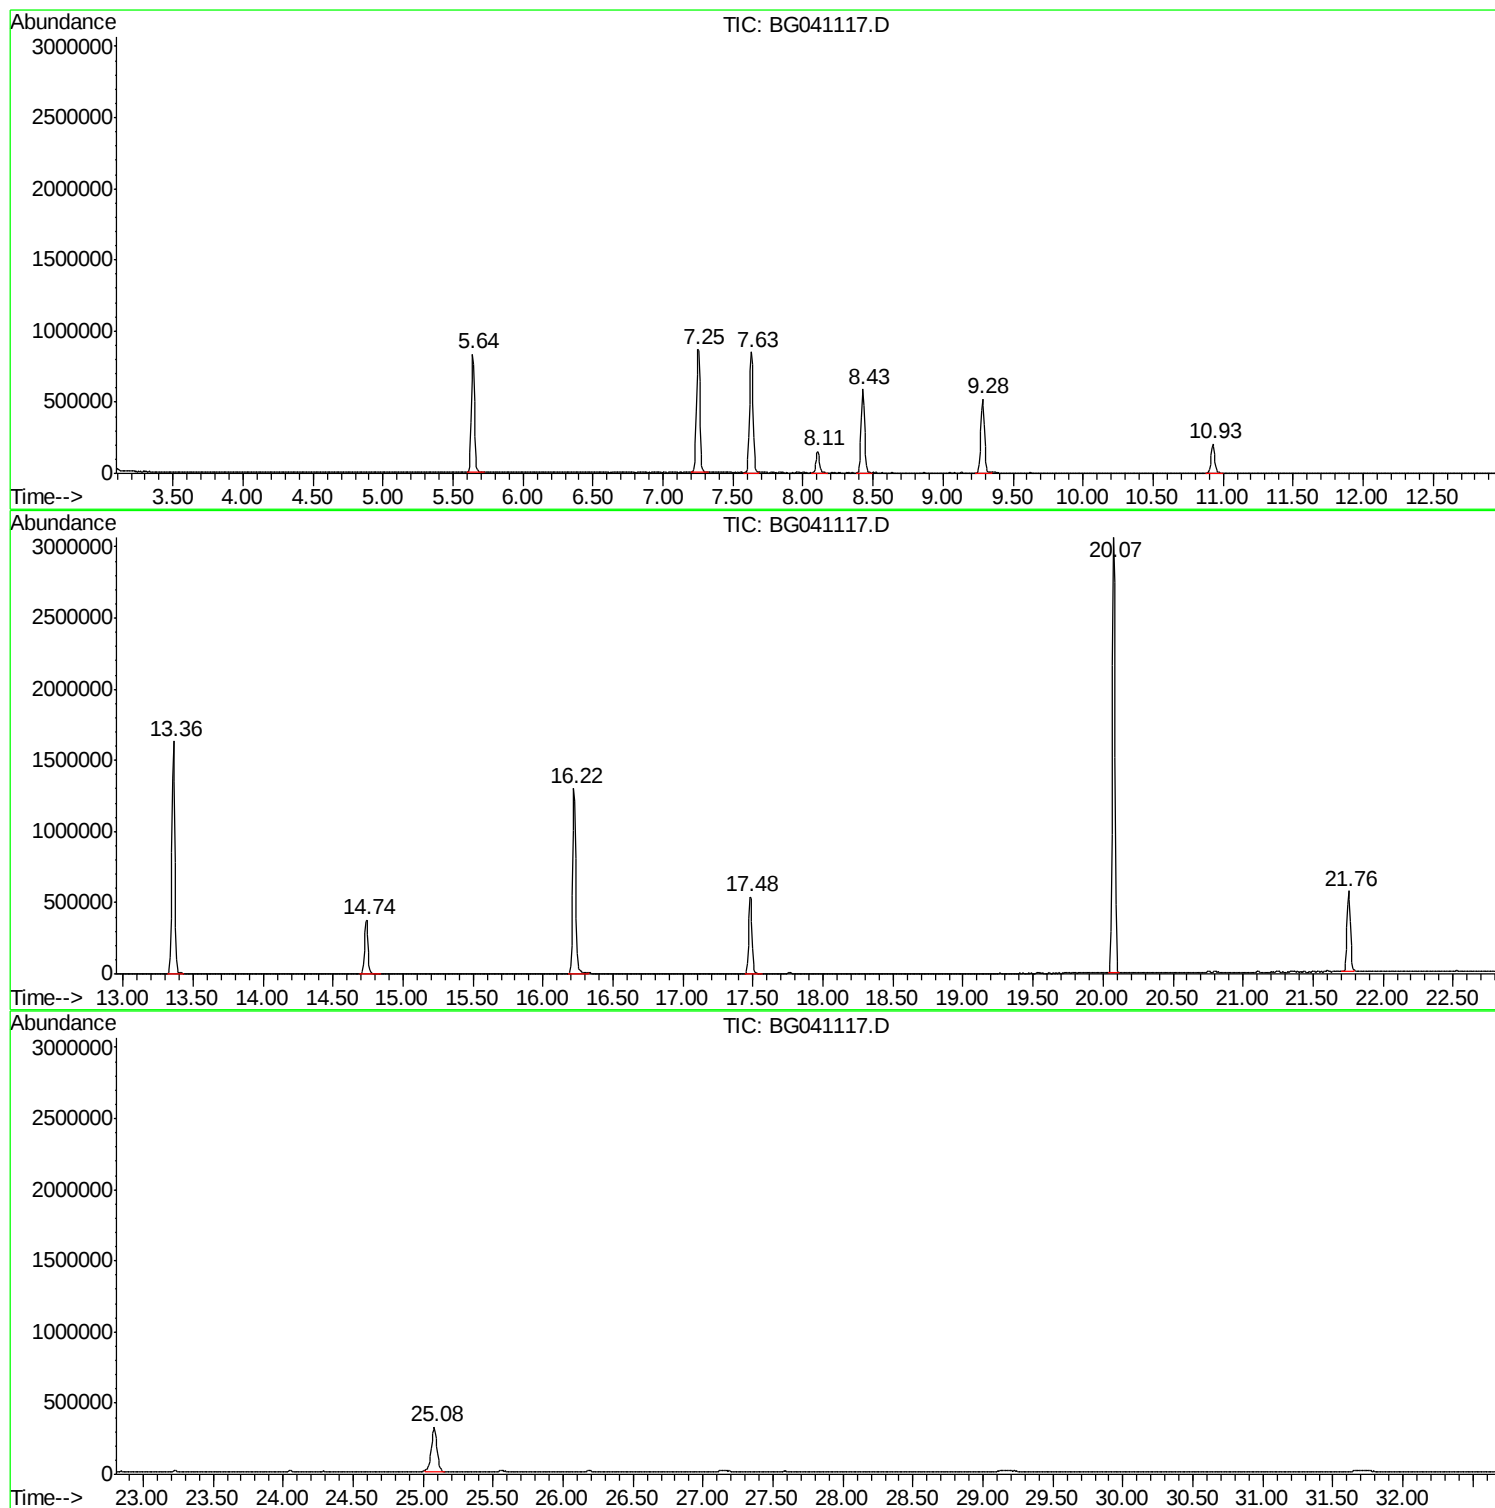

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060719\
Data File : BG041117.D
Acq On : 8 Jun 2019 3:29
Operator : HP/JU
Sample : PB120423BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120423BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.63	109.13 ng	1435170	1,4-Dichlorobenzene-d4	8.11

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		2H-Cyclopenta[d]pyridazine, 2-methyl-	132	C8H8N2	022291-85-6	22
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	22
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16

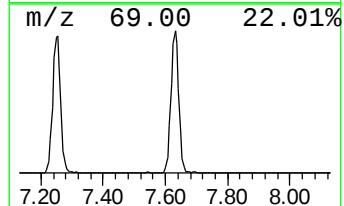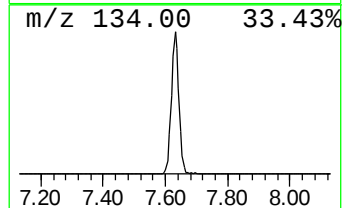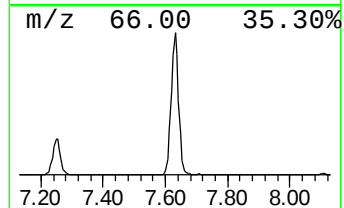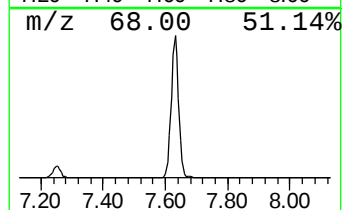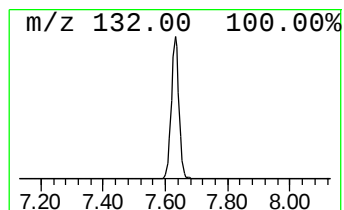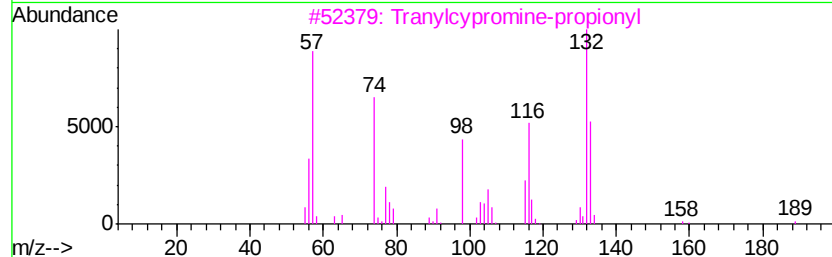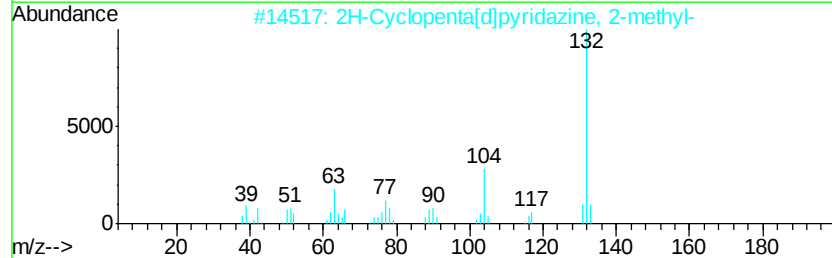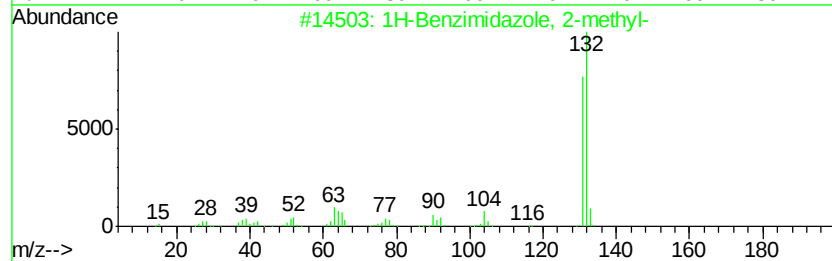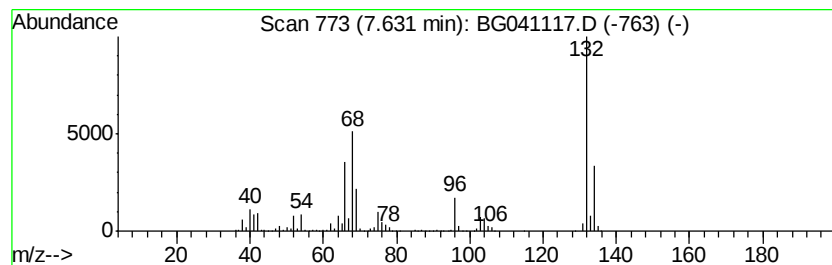

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060719\
Data File : BG041117.D
Acq On : 8 Jun 2019 3:29
Operator : HP/JU
Sample : PB120423BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120423BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.63	7.63	109.1	ng	1435170	1	8.11	263023	20.0