


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060719\
 Data File : BG041094.D
 Acq On : 7 Jun 2019 10:20
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

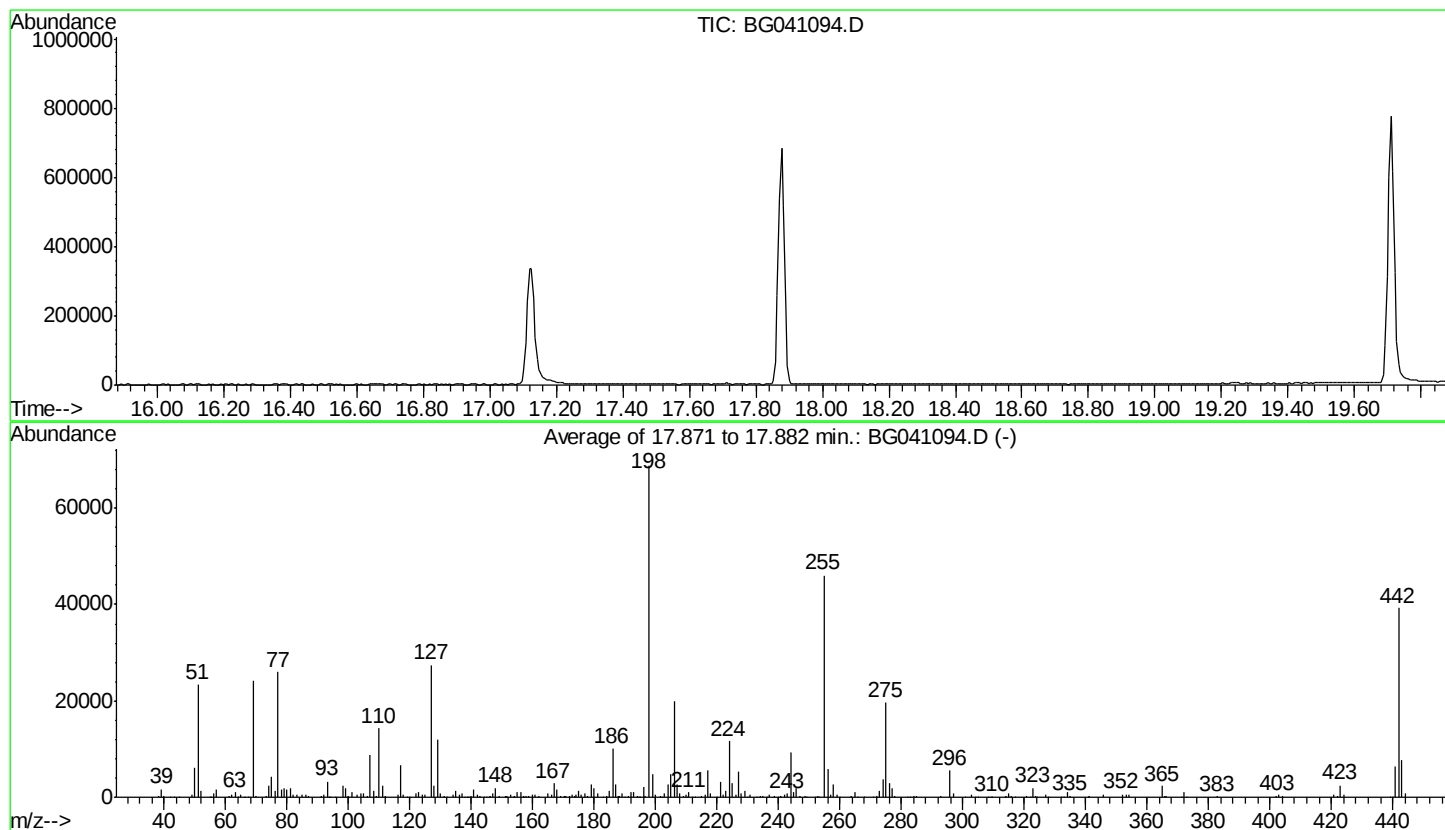

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	23325	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.1	24141	PASS
70	69	0.00	2	1.0	235	PASS
127	198	10	80	39.9	27440	PASS
197	198	0.00	2	0.3	175	PASS
198	198	100	100	100.0	68813	PASS
199	198	5	9	7.0	4821	PASS
275	198	10	60	28.5	19600	PASS
365	198	1	100	3.4	2339	PASS
441	198	0.01	100	9.3	6377	PASS
442	198	50	100	57.1	39314	PASS
443	442	15	24	19.8	7788	PASS