


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060719\
 Data File : BG041109.D
 Acq On : 7 Jun 2019 21:47
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

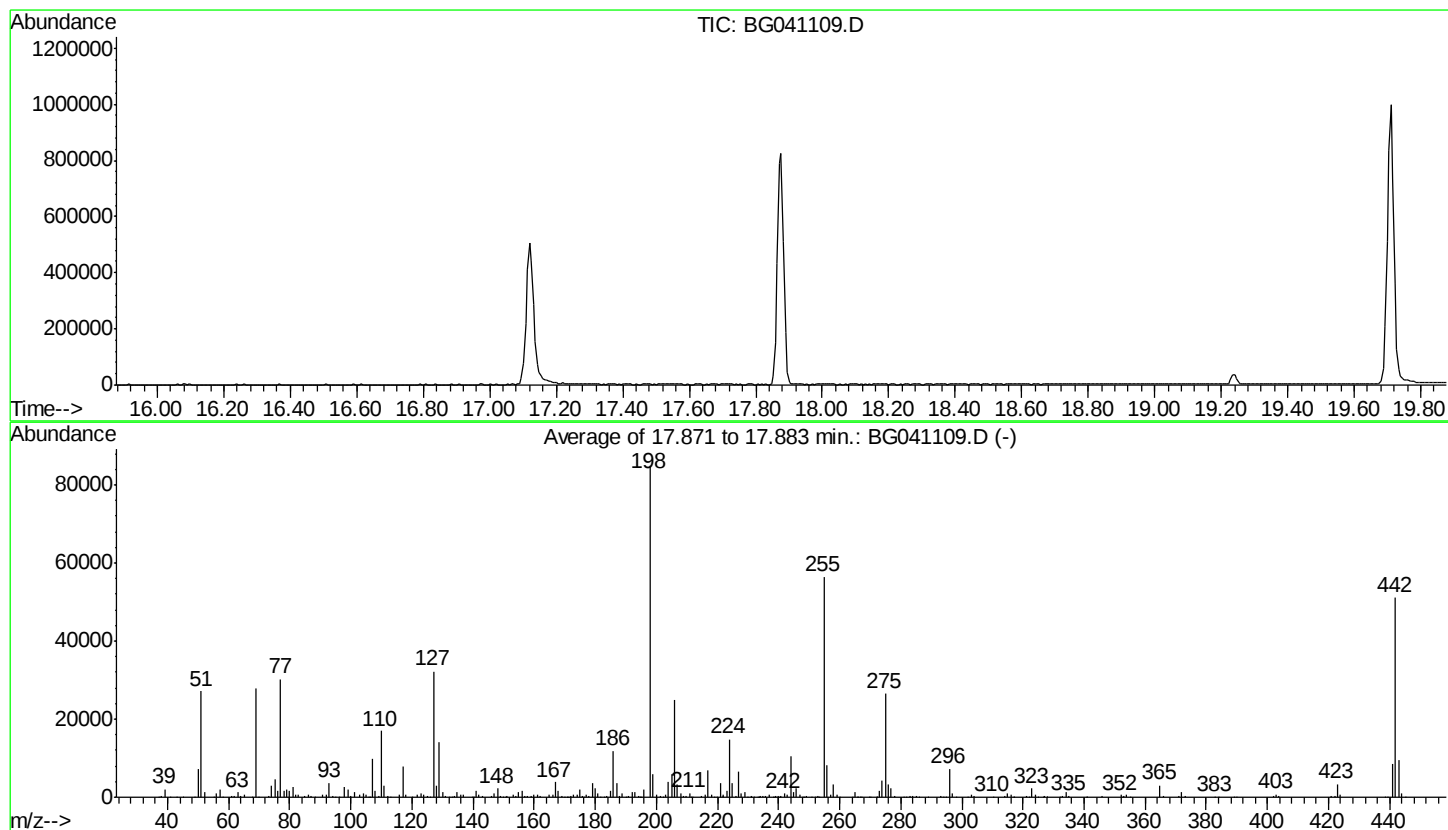

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	27177	PASS
68	69	0.00	2	0.3	86	PASS
69	198	0.00	100	32.8	27888	PASS
70	69	0.00	2	0.4	108	PASS
127	198	10	80	38.0	32282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84928	PASS
199	198	5	9	7.0	5941	PASS
275	198	10	60	31.2	26517	PASS
365	198	1	100	3.5	3012	PASS
441	198	0.01	100	10.1	8562	PASS
442	198	50	100	60.1	51037	PASS
443	442	15	24	19.0	9673	PASS