
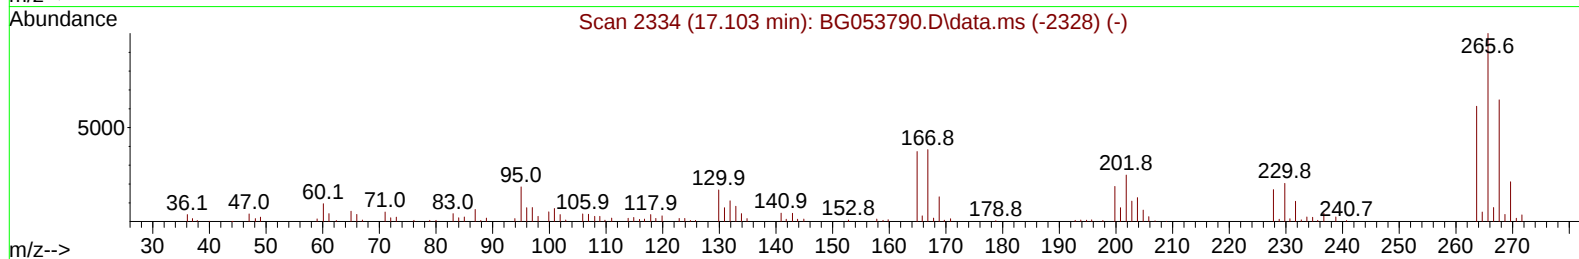
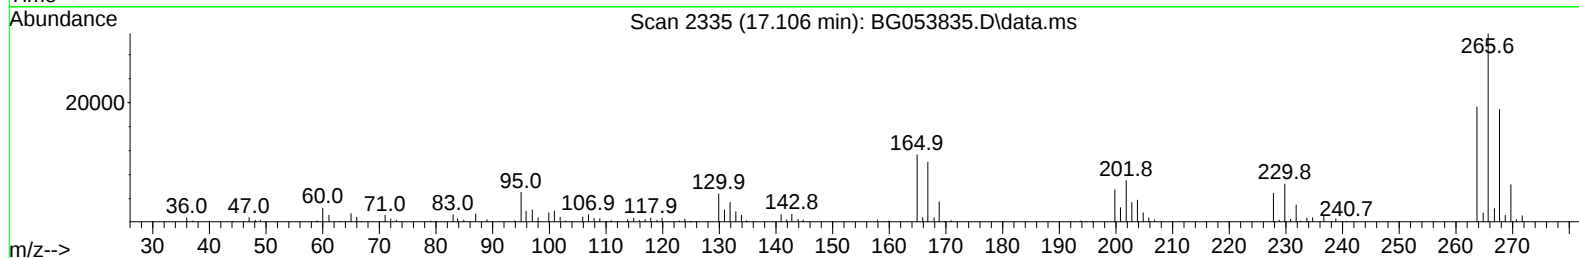


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
Data File : BG053835.D
Acq On : 7 Jun 2022 11:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 05:20:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

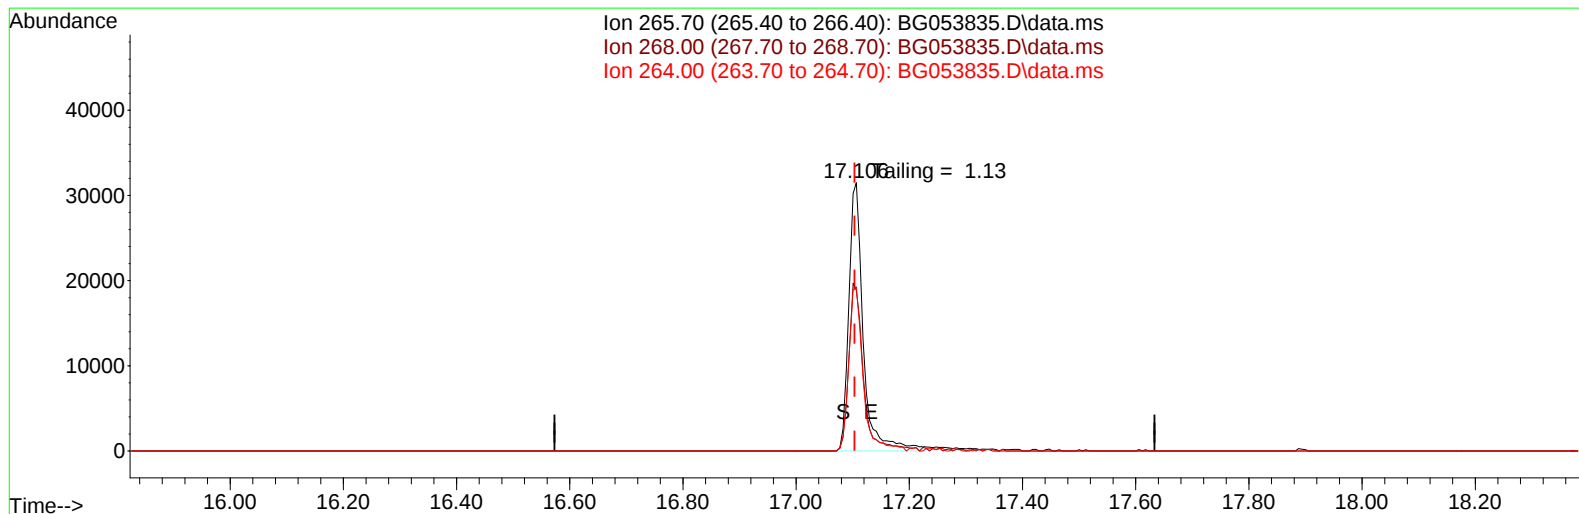

TIC: BG053835.D\data.ms

(70) Pentachlorophenol (C)




17.106min (+ 0.003) 27189.02 ng

response 55257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.82
264.00	66.20	61.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
Data File : BG053835.D
Acq On : 7 Jun 2022 11:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 05:20:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 23:22:27 2022
Response via : Initial Calibration

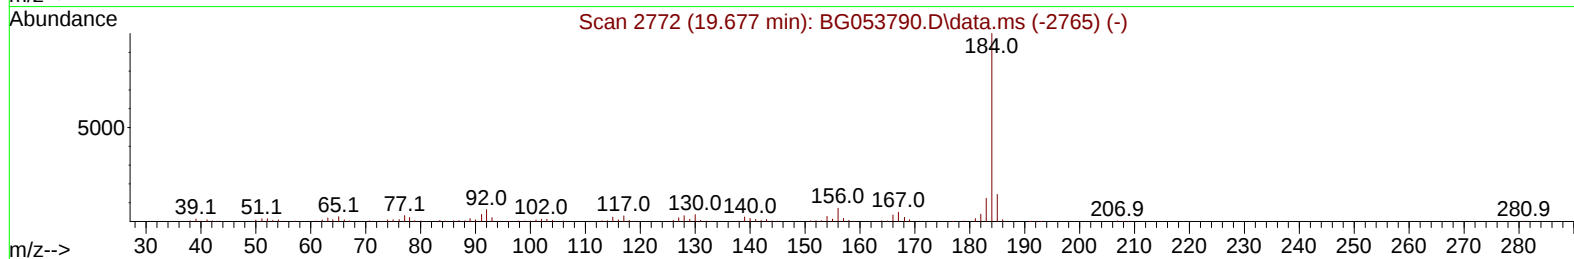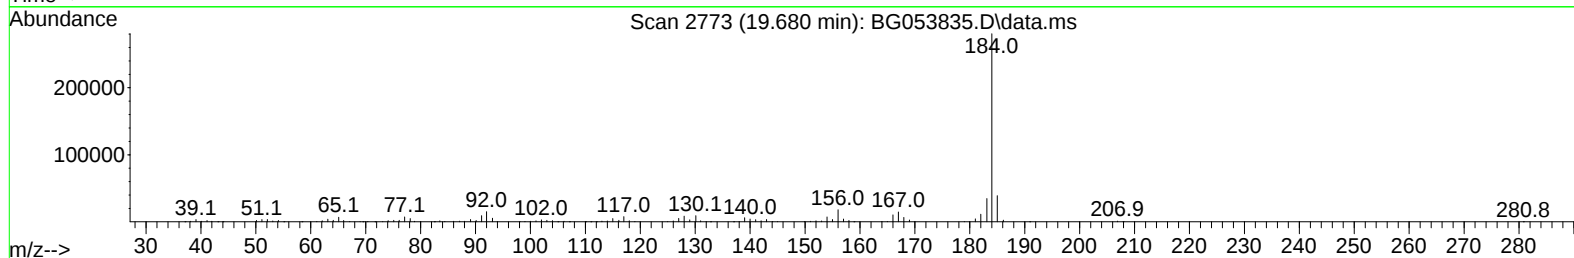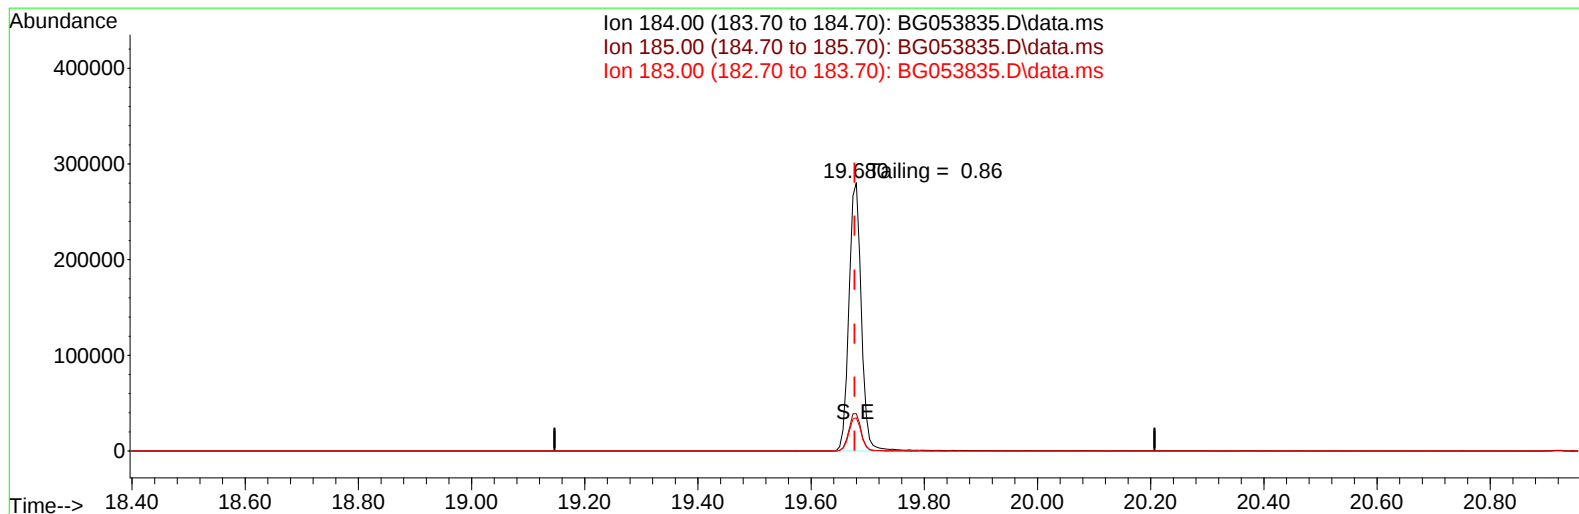

TIC: BG053835.D\data.ms

(77) Benzidine**19.680min (+ 0.003) 0.00 ng****response 426613**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.89
183.00	11.10	12.41
0.00	0.00	0.00