

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
 Data File : BG053839.D
 Acq On : 7 Jun 2022 15:04
 Operator : CG/JU
 Sample : N3189-03RX
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 20220423-AMENDED-COMPOSITE-CRX

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.586	199	204	215	rVB	45815	74640	3.59%	0.770%
2	5.197	298	308	319	rBV	1199892	2079892	100.00%	21.453%
3	5.649	380	385	392	rVB2	33834	56457	2.71%	0.582%
4	7.236	649	655	664	rVB	131975	231159	11.11%	2.384%
5	8.088	793	800	806	rBV	87600	152936	7.35%	1.577%
6	9.245	989	997	1008	rVB	270517	509915	24.52%	5.260%
7	9.609	1051	1059	1068	rBV	136793	270475	13.00%	2.790%
8	10.896	1269	1278	1285	rBV	116888	223340	10.74%	2.304%
9	13.340	1686	1694	1702	rBV	753483	1188175	57.13%	12.255%
10	13.464	1709	1715	1720	rBV	15544	26660	1.28%	0.275%
11	13.746	1756	1763	1771	rBV	27841	49889	2.40%	0.515%
12	14.615	1905	1911	1920	rBV2	26515	57557	2.77%	0.594%
13	14.715	1920	1928	1935	rVB	200431	347523	16.71%	3.585%
14	16.202	2175	2181	2190	rVB7	18261	39501	1.90%	0.407%
15	16.419	2212	2218	2229	rVB2	101624	189107	9.09%	1.951%
16	17.200	2345	2351	2358	rBV4	55016	102327	4.92%	1.055%
17	17.453	2388	2394	2399	rBV	280264	451012	21.68%	4.652%
18	17.494	2399	2401	2406	rVB	23318	32178	1.55%	0.332%
19	17.582	2413	2416	2422	rVB	12844	21529	1.04%	0.222%
20	18.381	2548	2552	2557	rBV6	15905	29745	1.43%	0.307%
21	19.357	2715	2718	2724	rVB2	36070	43645	2.10%	0.450%
22	19.509	2739	2744	2749	rBV	78224	112713	5.42%	1.163%
23	19.868	2801	2805	2813	rVB	81892	132009	6.35%	1.362%
24	20.062	2832	2838	2844	rBV	1422773	1905989	91.64%	19.659%
25	21.372	3057	3061	3070	rVB2	128553	200868	9.66%	2.072%
26	21.730	3115	3122	3128	rBV2	293036	571998	27.50%	5.900%
27	23.963	3496	3502	3510	rBV	36138	111452	5.36%	1.150%
28	25.003	3670	3679	3688	rBV2	163688	482356	23.19%	4.975%




Sum of corrected areas: 9695047

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
Data File : BG053839.D
Acq On : 7 Jun 2022 15:04
Operator : CG/JU
Sample : N3189-03RX
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20220423-AMENDED-COMPOSITE-CRX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

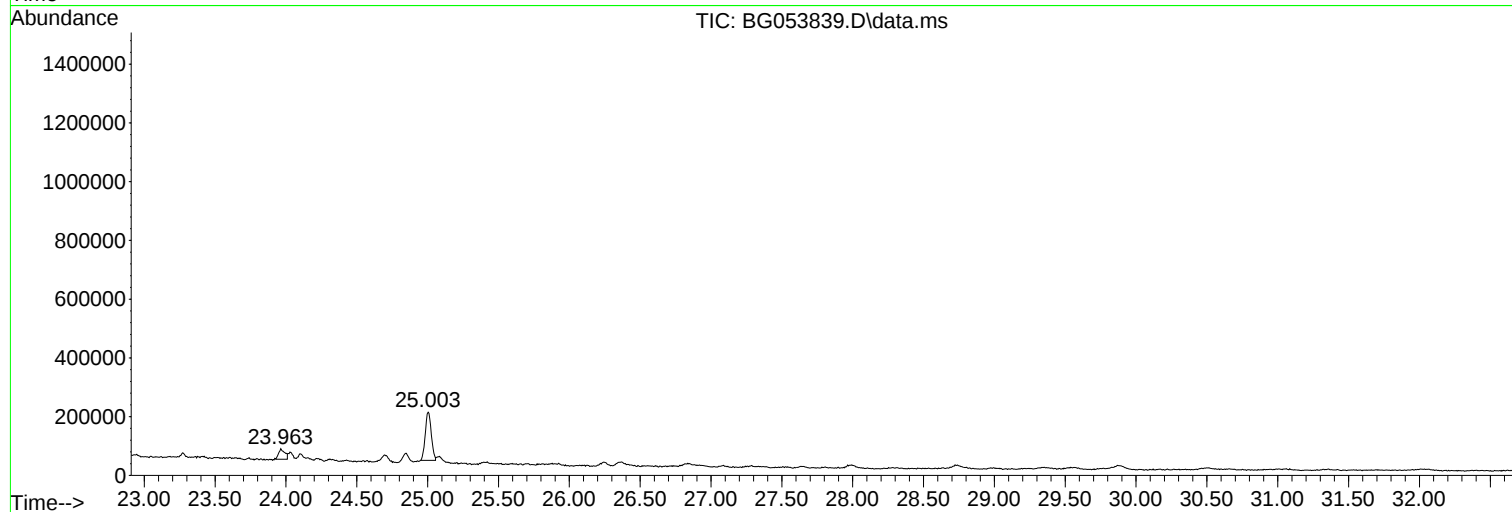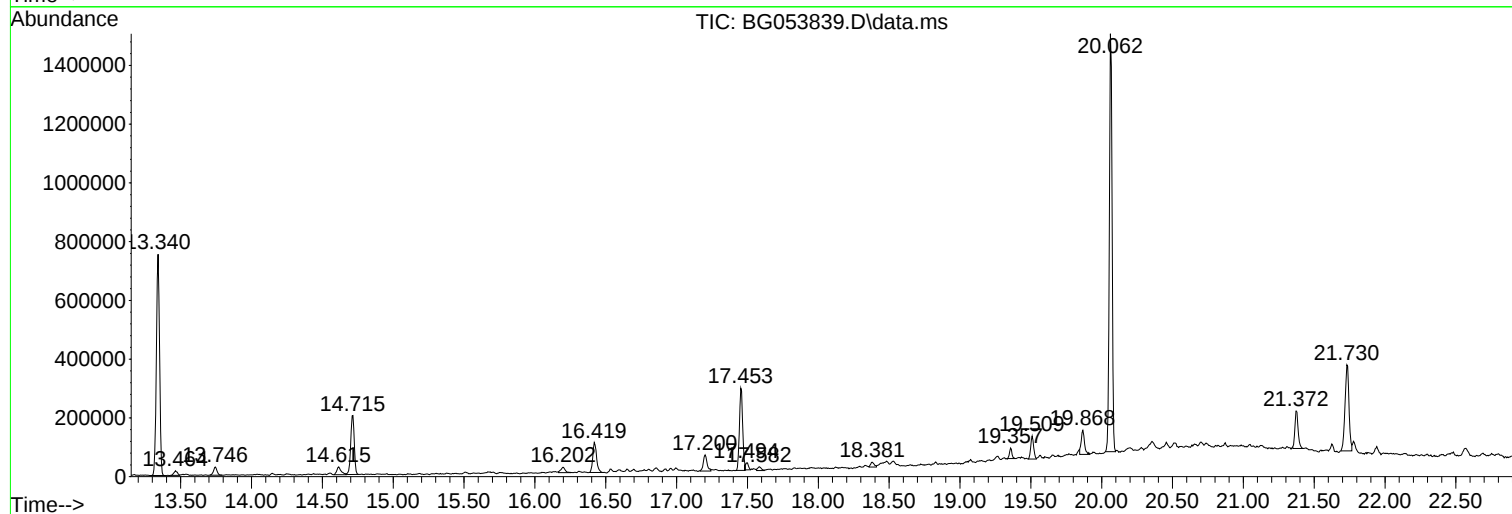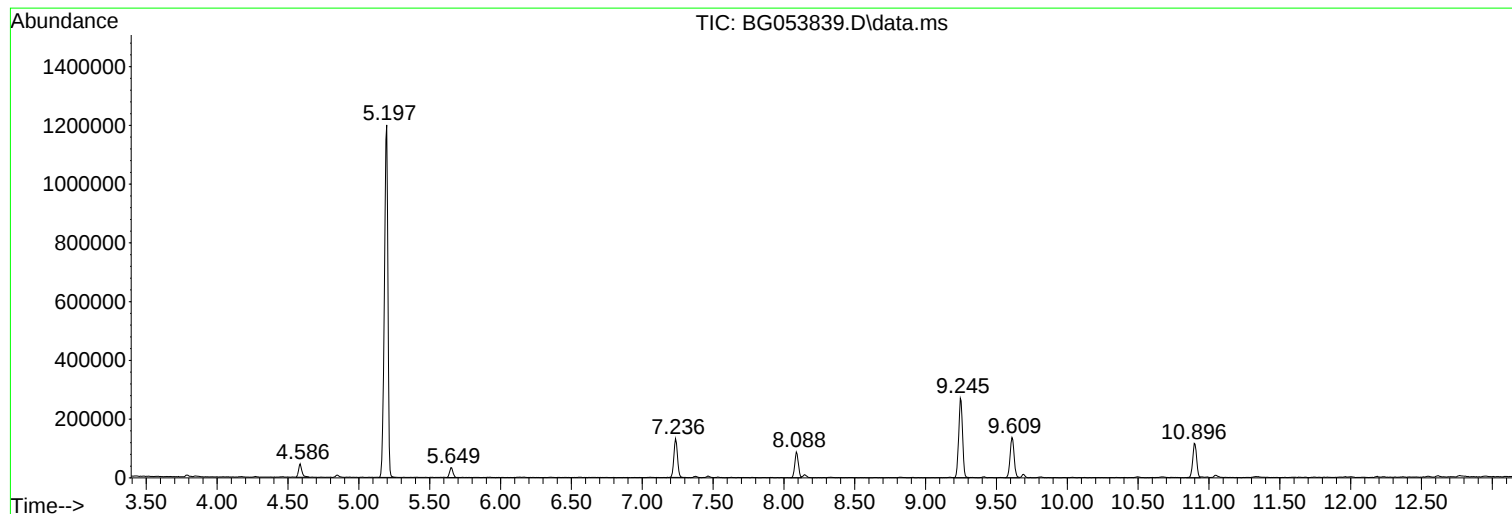

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
Data File : BG053839.D
Acq On : 7 Jun 2022 15:04
Operator : CG/JU
Sample : N3189-03RX
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20220423-AMENDED-COMPOSITE-CRX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
Data File : BG053839.D
Acq On : 7 Jun 2022 15:04
Operator : CG/JU
Sample : N3189-03RX
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
20220423-AMENDED-COMPOSITE-CRX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------