
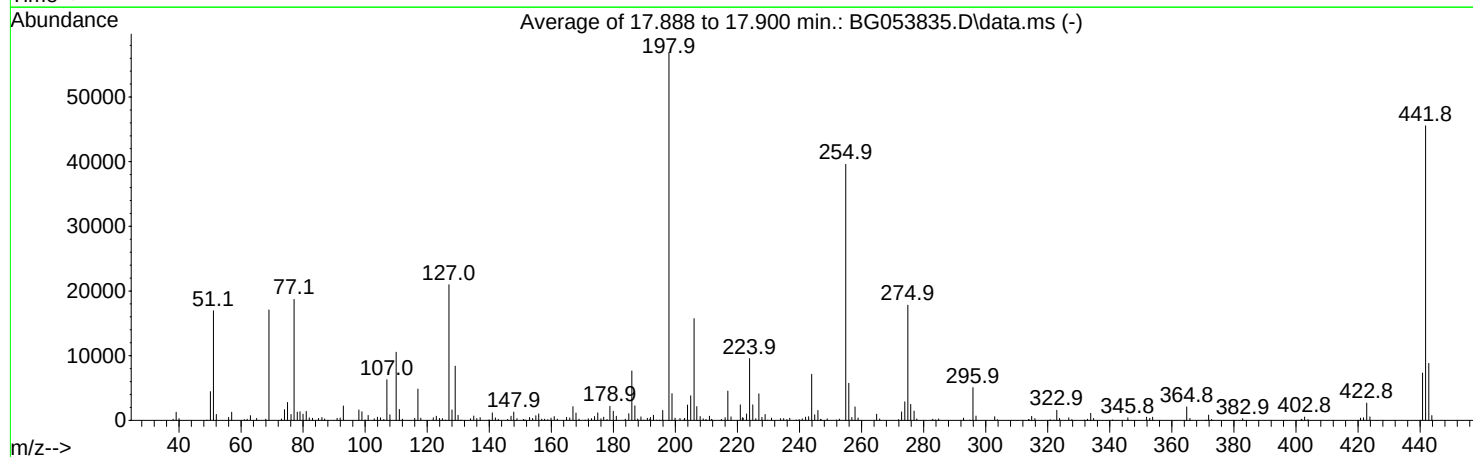


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
 Data File : BG053835.D
 Acq On : 7 Jun 2022 11:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

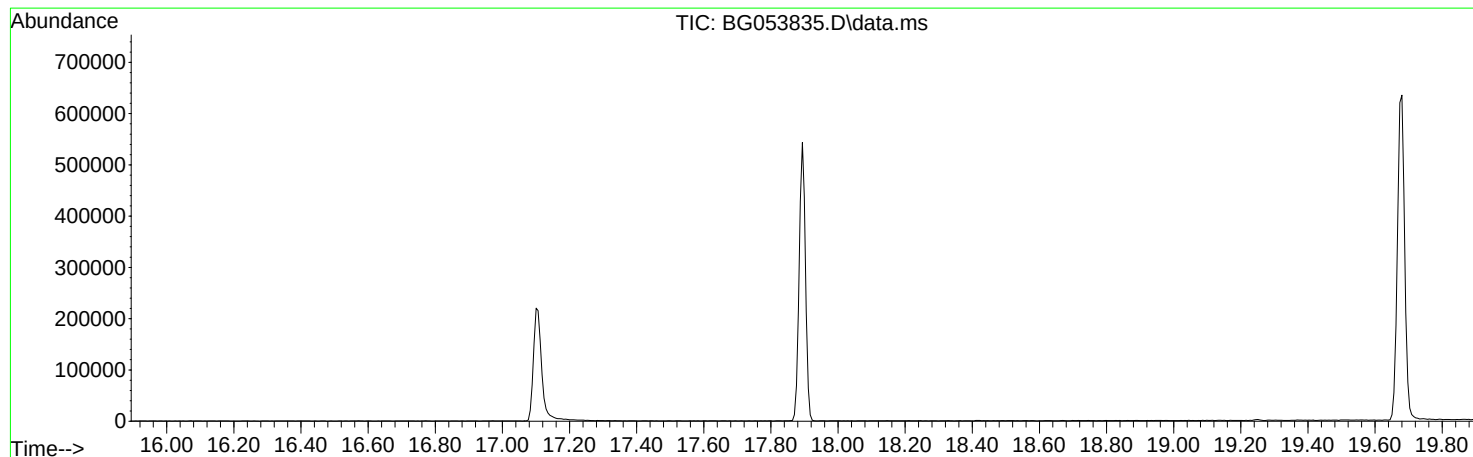




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	16953	PASS
68	69	0.00	2	1.2	203	PASS
69	198	0.00	100	30.0	17063	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.9	20981	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56880	PASS
199	198	5	9	7.3	4133	PASS
275	198	10	60	31.3	17821	PASS
365	198	1	100	3.6	2073	PASS
441	198	0.01	100	12.9	7315	PASS
442	442	50	100	100.0	45547	PASS
443	442	15	24	19.3	8800	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060722\
 Data File : BG053835.D
 Acq On : 7 Jun 2022 11:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 08 05:20:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 23:22:27 2022
 Response via : Initial Calibration

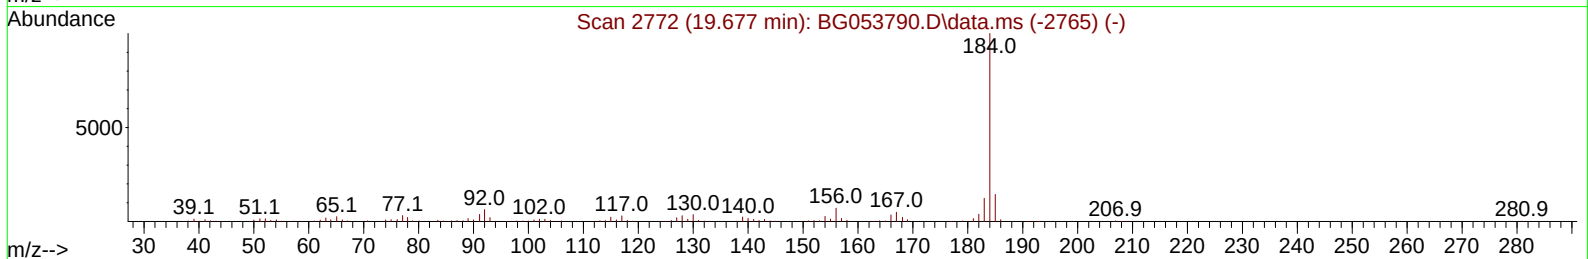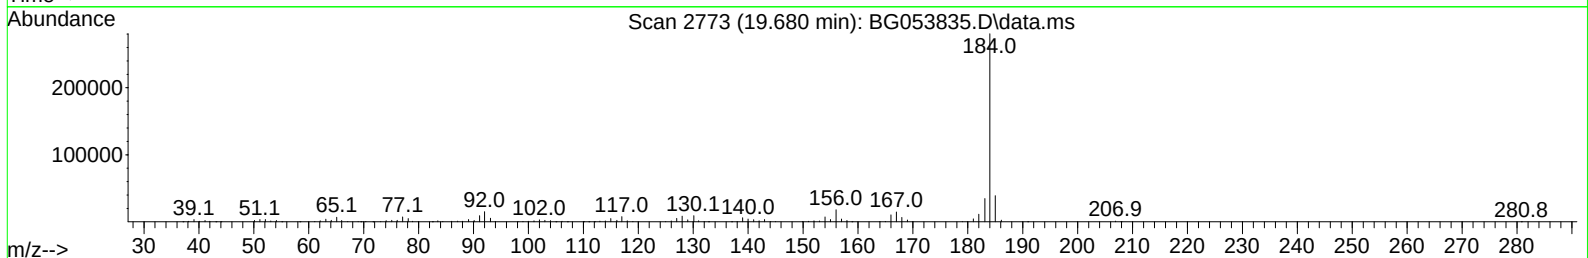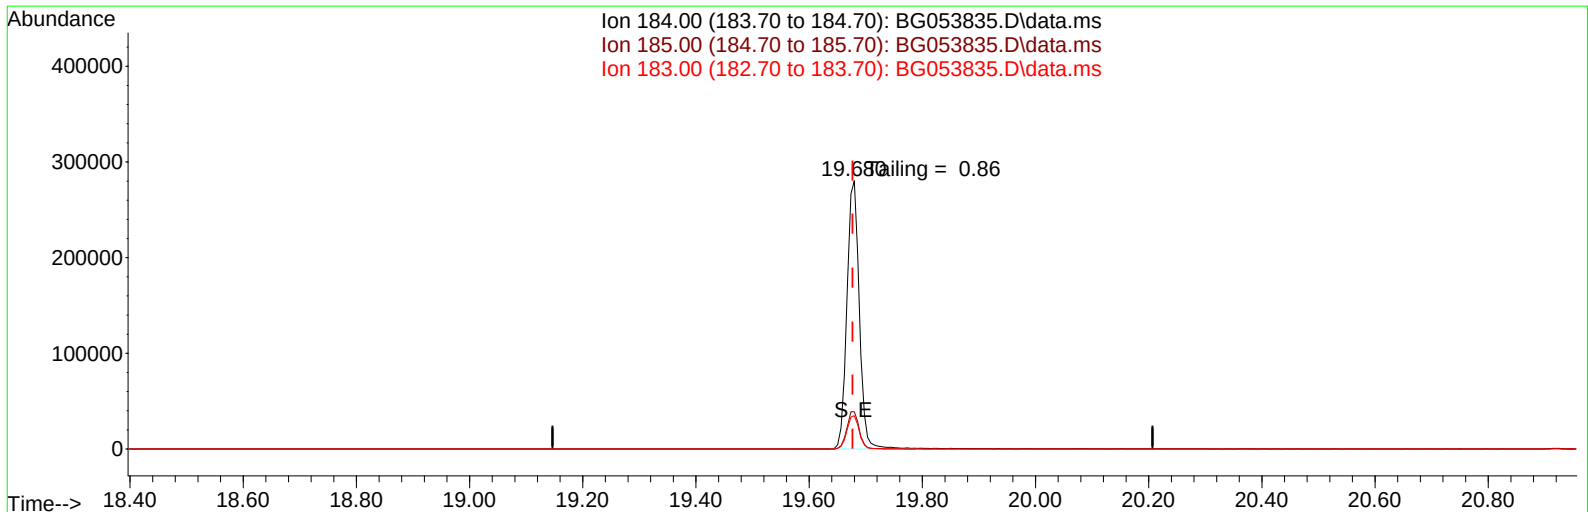

TIC: BG053835.D\data.ms

(77) Benzidine

19.680min (+ 0.003) 0.00 ng

response 426613

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.89
183.00	11.10	12.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2022	BNA_G	<u>BG053835.D</u>
Compound Name	Response	Retention Time
DDT	211933	20.92
DDD	1639	20.473
DDE	0	19.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1639	213572	0.77

Instrument :
BNA_G
ClientSampleId :
DFTPP