

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
 Data File : BG061532.D
 Acq On : 7 Jun 2024 14:07
 Operator : MA/JU
 Sample : PB161362BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	9	14	21	rVB	20126	31572	3.86%	0.397%
2	3.328	54	58	64	rVB3	4946	7400	0.90%	0.093%
3	3.734	122	127	138	rVV	70463	118695	14.50%	1.492%
4	4.069	181	184	188	rVB2	1117	1520	0.19%	0.019%
5	7.065	687	694	702	rVV	106542	176268	21.54%	2.216%
6	7.200	711	717	724	rBV	63016	105473	12.89%	1.326%
7	7.412	747	753	760	rBV	103871	166220	20.31%	2.090%
8	7.870	824	831	839	rVB	90232	149717	18.30%	1.882%
9	8.599	949	955	965	rBV2	132368	220511	26.95%	2.773%
10	9.034	1019	1029	1036	rBV	108367	185178	22.63%	2.328%
11	9.756	1145	1152	1160	rVB	95588	167337	20.45%	2.104%
12	10.309	1239	1246	1257	rBV	137337	239410	29.26%	3.010%
13	10.667	1300	1307	1315	rBV	129170	225843	27.60%	2.840%
14	10.808	1324	1331	1342	rVB	132971	237203	28.99%	2.982%
15	12.265	1574	1579	1583	rBB3	1819	3229	0.39%	0.041%
16	13.922	1855	1861	1869	rBV	261899	370679	45.30%	4.661%
17	14.210	1903	1910	1917	rBV	267730	419070	51.21%	5.269%
18	14.515	1955	1962	1969	rVB	222817	336279	41.09%	4.228%
19	14.762	1998	2004	2015	rBV	64130	127000	15.52%	1.597%
20	15.514	2125	2132	2140	rBV	349205	525809	64.25%	6.611%
21	15.655	2151	2156	2166	rBV	84312	131012	16.01%	1.647%
22	15.749	2171	2172	2175	rVB	1375	1041	0.13%	0.013%
23	16.678	2326	2330	2332	rBV	712	906	0.11%	0.011%
24	17.059	2391	2395	2397	rBV2	728	1185	0.14%	0.015%
25	17.265	2424	2430	2437	rBV	292577	419677	51.29%	5.277%
26	17.365	2441	2447	2456	rVB	399785	591652	72.30%	7.439%
27	17.765	2509	2515	2516	rBV	1057	991	0.12%	0.012%
28	18.164	2579	2583	2586	rVV2	1046	1668	0.20%	0.021%
29	18.340	2610	2613	2616	rVB3	1276	1037	0.13%	0.013%
30	18.822	2694	2695	2698	rVV3	1035	1127	0.14%	0.014%
31	18.851	2698	2700	2703	rVV3	1284	1526	0.19%	0.019%
32	18.951	2715	2717	2721	rVB2	1253	1674	0.20%	0.021%
33	18.992	2721	2724	2725	rBV2	1118	1287	0.16%	0.016%
34	19.039	2731	2732	2735	rVB2	1081	928	0.11%	0.012%
35	19.069	2735	2737	2739	rBV	1380	1408	0.17%	0.018%
36	19.227	2758	2764	2767	rVV2	6796	8359	1.02%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
 Data File : BG061532.D
 Acq On : 7 Jun 2024 14:07
 Operator : MA/JU
 Sample : PB161362BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

37	19.292	2772	2775	2780	rBV2	4686	8118	0.99%	0.102%
38	19.333	2780	2782	2784	rVV2	1650	2034	0.25%	0.026%
39	19.410	2794	2795	2798	rBV3	1592	1301	0.16%	0.016%
40	19.586	2823	2825	2827	rVB3	2265	1969	0.24%	0.025%
41	19.627	2829	2832	2833	rBV3	1674	1735	0.21%	0.022%
42	19.662	2833	2838	2844	rBV	544081	721615	88.18%	9.073%
43	19.803	2861	2862	2864	rBV	1176	857	0.10%	0.011%
44	19.833	2865	2867	2869	rVV3	2098	1586	0.19%	0.020%
45	19.856	2869	2871	2872	rVV2	1803	989	0.12%	0.012%
46	19.874	2872	2874	2876	rVV3	1414	996	0.12%	0.013%
47	19.921	2880	2882	2883	rBV2	1157	975	0.12%	0.012%
48	19.956	2887	2888	2890	rBV2	1027	1025	0.13%	0.013%
49	20.044	2901	2903	2904	rBV	1785	984	0.12%	0.012%
50	20.062	2904	2906	2908	rVB3	1978	1687	0.21%	0.021%
51	20.085	2908	2910	2911	rBV2	2163	1379	0.17%	0.017%
52	20.168	2922	2924	2927	rBV3	2731	2152	0.26%	0.027%
53	20.197	2927	2929	2930	rBV2	2828	1953	0.24%	0.025%
54	20.232	2933	2935	2936	rVV2	1612	1023	0.13%	0.013%
55	20.309	2946	2948	2950	rBV3	2943	3067	0.37%	0.039%
56	20.326	2950	2951	2952	rBV	2301	1155	0.14%	0.015%
57	20.397	2961	2963	2965	rBV3	2263	1815	0.22%	0.023%
58	20.479	2975	2977	2979	rBV3	2581	2187	0.27%	0.027%
59	20.555	2986	2990	2993	rBV6	2868	3809	0.47%	0.048%
60	20.620	3000	3001	3002	rBV	4441	2667	0.33%	0.034%
61	20.696	3012	3014	3017	rVB4	5478	3715	0.45%	0.047%
62	20.743	3020	3022	3023	rBV2	2039	898	0.11%	0.011%
63	20.761	3023	3025	3026	rVB2	2935	1613	0.20%	0.020%
64	20.773	3026	3027	3031	rBV4	3302	3301	0.40%	0.042%
65	20.808	3031	3033	3036	rVB4	3965	3331	0.41%	0.042%
66	20.902	3047	3049	3051	rBV2	3478	3687	0.45%	0.046%
67	20.984	3061	3063	3064	rBV2	3072	1912	0.23%	0.024%
68	21.020	3067	3069	3072	rVB4	2950	2585	0.32%	0.033%
69	21.184	3094	3097	3101	rVV2	12736	12677	1.55%	0.159%
70	21.231	3103	3105	3106	rBV2	3699	2565	0.31%	0.032%
71	21.401	3132	3134	3135	rBV2	3654	3216	0.39%	0.040%
72	21.531	3148	3156	3163	rBV	341334	548072	66.98%	6.891%
73	21.719	3183	3188	3192	rVB3	13810	21591	2.64%	0.271%
74	22.048	3242	3244	3246	rBV3	4159	4820	0.59%	0.061%
75	22.300	3283	3287	3292	rVB5	19338	31000	3.79%	0.390%
76	22.383	3299	3301	3304	rBV4	4723	4610	0.56%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
 Data File : BG061532.D
 Acq On : 7 Jun 2024 14:07
 Operator : MA/JU
 Sample : PB161362BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

77	22.436	3309	3310	3311	rBV	4234	1827	0.22%	0.023%
78	22.712	3355	3357	3359	rBV3	4730	3928	0.48%	0.049%
79	22.864	3381	3383	3384	rBV	3914	2493	0.30%	0.031%
80	22.964	3395	3400	3406	rVB7	15209	31535	3.85%	0.397%
81	23.023	3408	3410	3412	rVB3	4207	2336	0.29%	0.029%
82	23.722	3525	3529	3537	rVB10	13685	34243	4.18%	0.431%
83	23.963	3568	3570	3572	rBV3	3882	2614	0.32%	0.033%
84	24.421	3639	3648	3663	rBV2	309793	818319	100.00%	10.289%
85	24.633	3675	3684	3694	rBV2	209311	570016	69.66%	7.167%
86	24.868	3722	3724	3725	rBV2	4623	3435	0.42%	0.043%
87	25.256	3788	3790	3791	rBV2	4133	2646	0.32%	0.033%
88	25.497	3829	3831	3833	rBV3	5212	4627	0.57%	0.058%
89	25.702	3861	3866	3874	rVB6	16558	37871	4.63%	0.476%
90	26.824	4055	4057	4062	rBV4	3969	5191	0.63%	0.065%
91	28.481	4337	4339	4341	rBV3	4510	5333	0.65%	0.067%
92	28.840	4398	4400	4401	rBV	4954	3257	0.40%	0.041%
93	29.433	4499	4501	4504	rVB4	4482	3893	0.48%	0.049%
94	29.463	4504	4506	4509	rBV4	4617	4330	0.53%	0.054%
95	30.109	4614	4616	4619	rBV4	4347	4930	0.60%	0.062%
96	31.448	4842	4844	4846	rBV3	4268	4531	0.55%	0.057%
97	31.636	4874	4876	4877	rVB2	4114	2044	0.25%	0.026%
98	32.083	4950	4952	4953	rVB2	6495	3194	0.39%	0.040%
99	32.101	4953	4955	4956	rBV2	3538	2281	0.28%	0.029%
100	32.618	5042	5043	5044	rBV	4383	1817	0.22%	0.023%



Sum of corrected areas: 7953253

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
Data File : BG061532.D
Acq On : 7 Jun 2024 14:07
Operator : MA/JU
Sample : PB161362BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

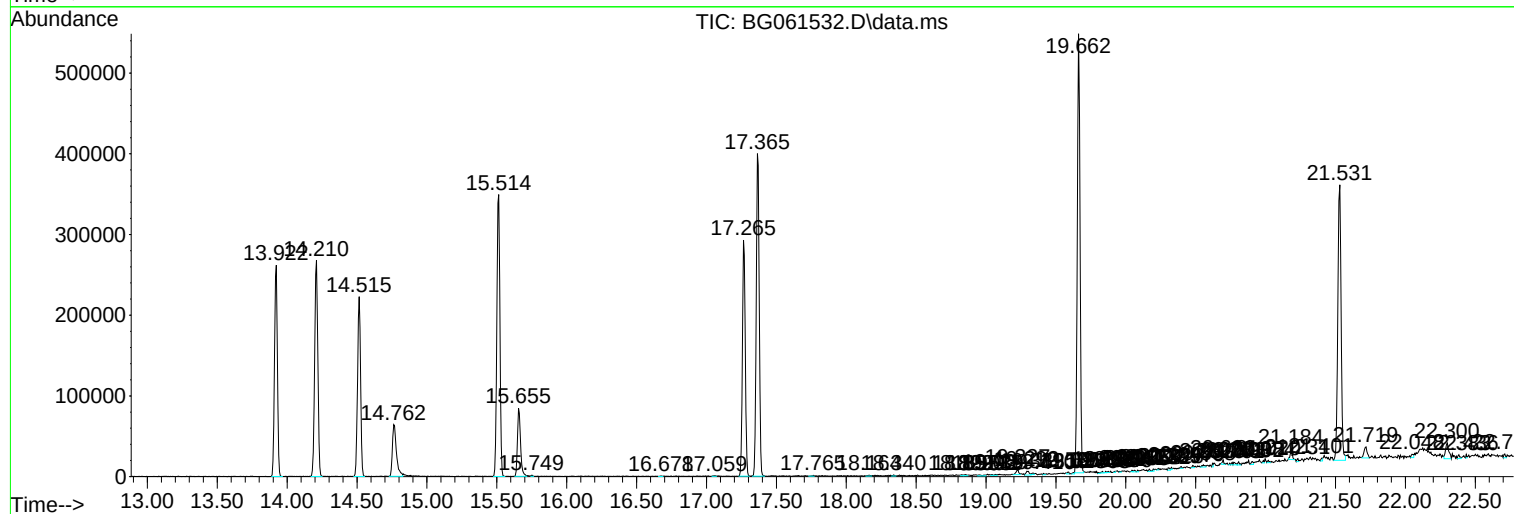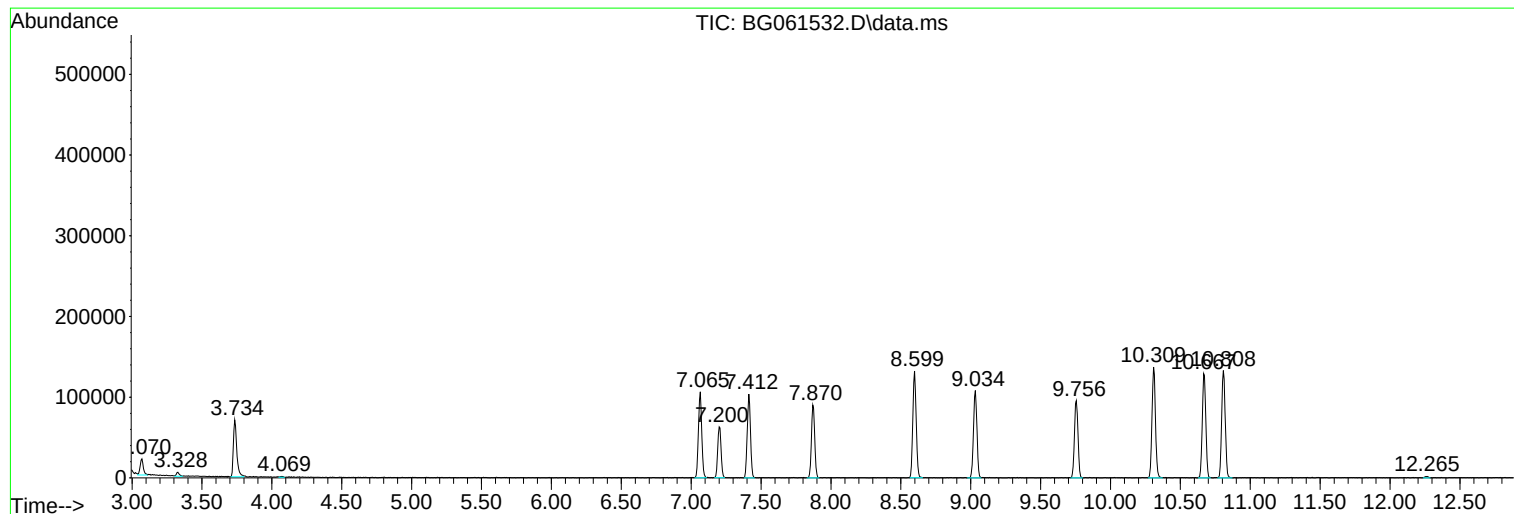

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
Data File : BG061532.D
Acq On : 7 Jun 2024 14:07
Operator : MA/JU
Sample : PB161362BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK362










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.070	4.22 ng/ul	31572	1,4-Dichlorobenzene-d4	7.870

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	9
4			2-Acetamido-N-methylacetamide	130	C5H10N2O2	007606-79-3	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

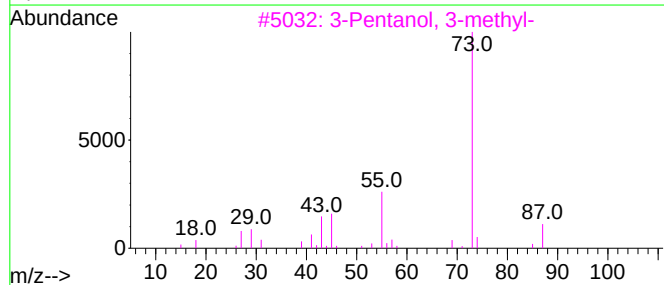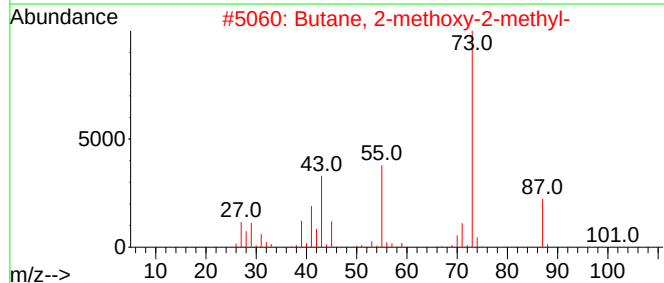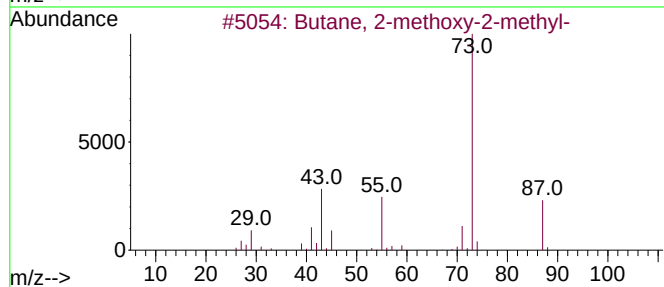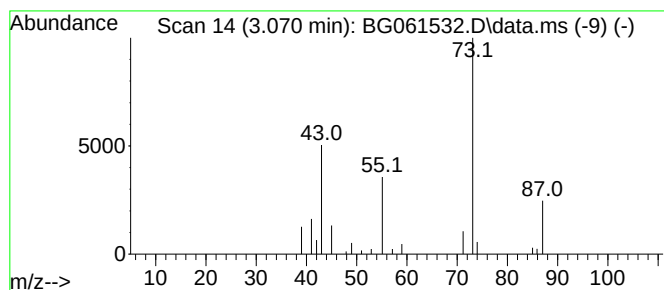

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
Data File : BG061532.D
Acq On : 7 Jun 2024 14:07
Operator : MA/JU
Sample : PB161362BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK362

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.070	4.2	ng/u1	31572	1	7.870	149717	20.0