

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
 Data File : BG061538.D
 Acq On : 7 Jun 2024 18:16
 Operator : MA/JU
 Sample : PB161251BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.065	9	13	22	rVB	20739	31574	3.22%	0.347%
2	3.323	53	57	61	rBV2	5981	7560	0.77%	0.083%
3	3.494	83	86	91	rVB2	597	1098	0.11%	0.012%
4	3.735	122	127	141	rBV	88391	147907	15.07%	1.623%
5	4.069	178	184	189	rBV3	5129	7853	0.80%	0.086%
6	4.510	257	259	265	rVB	639	1065	0.11%	0.012%
7	4.575	265	270	273	rBV2	552	1169	0.12%	0.013%
8	7.060	687	693	704	rBV	134397	227173	23.14%	2.493%
9	7.201	710	717	725	rVB	86672	134969	13.75%	1.481%
10	7.413	746	753	762	rBB	124463	211085	21.50%	2.317%
11	7.871	825	831	838	rVB	97959	157444	16.04%	1.728%
12	8.599	947	955	967	rVB	156589	277744	28.29%	3.048%
13	9.028	1020	1028	1036	rBB	131429	228868	23.31%	2.512%
14	9.751	1144	1151	1161	rVB	119825	211175	21.51%	2.318%
15	10.309	1238	1246	1258	rBV	165848	302802	30.84%	3.323%
16	10.668	1299	1307	1315	rVB	130921	231453	23.57%	2.540%
17	10.809	1323	1331	1340	rBV	162553	287286	29.26%	3.153%
18	12.260	1573	1578	1584	rVB	2015	3308	0.34%	0.036%
19	13.917	1854	1860	1868	rBV	302396	440032	44.82%	4.830%
20	14.205	1902	1909	1917	rBV	326417	513961	52.35%	5.641%
21	14.516	1955	1962	1968	rBV	223253	346654	35.31%	3.805%
22	14.763	1997	2004	2018	rBV	78816	153339	15.62%	1.683%
23	14.857	2018	2020	2028	rVV2	1858	3221	0.33%	0.035%
24	15.509	2125	2131	2139	rVB	440505	636374	64.82%	6.984%
25	15.656	2151	2156	2163	rBV2	100514	152866	15.57%	1.678%
26	15.744	2170	2171	2176	rVB2	1770	1729	0.18%	0.019%
27	17.042	2390	2392	2399	rBV2	684	1231	0.13%	0.014%
28	17.266	2424	2430	2436	rBV	302883	433512	44.16%	4.758%
29	17.366	2440	2447	2455	rBV2	473505	699411	71.24%	7.676%
30	18.887	2703	2706	2708	rBV2	1071	1030	0.10%	0.011%
31	19.140	2746	2749	2752	rBV2	1003	1373	0.14%	0.015%
32	19.175	2752	2755	2757	rVB	884	1074	0.11%	0.012%
33	19.222	2760	2763	2770	rVB3	6938	10121	1.03%	0.111%
34	19.299	2770	2776	2780	rBV4	6745	10640	1.08%	0.117%
35	19.328	2780	2781	2783	rVV	1285	995	0.10%	0.011%
36	19.346	2783	2784	2787	rVB	1724	1330	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
 Data File : BG061538.D
 Acq On : 7 Jun 2024 18:16
 Operator : MA/JU
 Sample : PB161251BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

37	19.493	2806	2809	2811	rBV4	1146	1593	0.16%	0.017%
38	19.516	2811	2813	2815	rVV	1541	1564	0.16%	0.017%
39	19.569	2818	2822	2824	rVV3	1856	2771	0.28%	0.030%
40	19.587	2824	2825	2827	rVV2	2964	1361	0.14%	0.015%
41	19.663	2831	2838	2849	rVV	619508	849056	86.48%	9.319%
42	19.757	2851	2854	2856	rBV4	2017	1906	0.19%	0.021%
43	19.786	2858	2859	2861	rBV2	2038	1056	0.11%	0.012%
44	19.992	2890	2894	2896	rVB5	1782	2191	0.22%	0.024%
45	20.068	2905	2907	2908	rBV2	1977	1455	0.15%	0.016%
46	20.080	2908	2909	2912	rVB3	2236	2068	0.21%	0.023%
47	20.115	2914	2915	2918	rVB2	2656	1469	0.15%	0.016%
48	20.145	2918	2920	2922	rBV3	2662	1772	0.18%	0.019%
49	20.174	2922	2925	2926	rBV2	2522	2346	0.24%	0.026%
50	20.286	2942	2944	2946	rVB2	2259	1774	0.18%	0.019%
51	20.315	2946	2949	2950	rBV3	3654	3007	0.31%	0.033%
52	20.344	2952	2954	2956	rVV3	2013	1770	0.18%	0.019%
53	20.368	2956	2958	2961	rVB4	2093	2253	0.23%	0.025%
54	20.403	2961	2964	2965	rBV3	2096	1974	0.20%	0.022%
55	20.515	2980	2983	2986	rBV5	2803	3633	0.37%	0.040%
56	20.544	2986	2988	2989	rBV2	1794	1602	0.16%	0.018%
57	20.562	2989	2991	2992	rVV2	1926	1169	0.12%	0.013%
58	20.673	3006	3010	3012	rBV5	4267	5224	0.53%	0.057%
59	20.967	3058	3060	3062	rBV3	3137	2250	0.23%	0.025%
60	21.008	3065	3067	3068	rBV2	3029	1517	0.15%	0.017%
61	21.055	3073	3075	3077	rBV3	5539	4340	0.44%	0.048%
62	21.114	3083	3085	3088	rBV4	4238	3936	0.40%	0.043%
63	21.179	3094	3096	3097	rBV2	3819	1689	0.17%	0.019%
64	21.525	3149	3155	3161	rBV2	333953	539231	54.92%	5.918%
65	21.708	3183	3186	3190	rBV6	7036	9305	0.95%	0.102%
66	22.219	3271	3273	3274	rBV2	3553	2413	0.25%	0.026%
67	22.295	3284	3286	3290	rVB5	8799	8881	0.90%	0.097%
68	22.360	3296	3297	3299	rVB2	4625	3214	0.33%	0.035%
69	22.466	3314	3315	3320	rBV5	5390	5694	0.58%	0.062%
70	22.642	3344	3345	3348	rBV3	4936	5096	0.52%	0.056%
71	22.795	3369	3371	3372	rBV2	4109	2439	0.25%	0.027%
72	23.241	3445	3447	3448	rBV2	3593	2054	0.21%	0.023%
73	23.359	3465	3467	3468	rBV2	3292	2412	0.25%	0.026%
74	23.729	3525	3530	3536	rVB7	12309	25822	2.63%	0.283%
75	23.817	3543	3545	3547	rBV3	4089	3257	0.33%	0.036%
76	24.422	3637	3648	3666	rBV	350836	981789	100.00%	10.776%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
 Data File : BG061538.D
 Acq On : 7 Jun 2024 18:16
 Operator : MA/JU
 Sample : PB161251BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

77	24.628	3674	3683	3699	rVB2	209569	596218	60.73%	6.544%
78	25.068	3756	3758	3759	rVB2	5087	3157	0.32%	0.035%
79	25.098	3759	3763	3766	rBV4	4795	6815	0.69%	0.075%
80	25.227	3783	3785	3788	rBV4	4871	4600	0.47%	0.050%
81	25.703	3859	3866	3877	rVB9	11697	33947	3.46%	0.373%
82	25.838	3887	3889	3891	rBV3	4873	3831	0.39%	0.042%
83	25.856	3891	3892	3893	rBV	3259	1521	0.15%	0.017%
84	25.932	3901	3905	3906	rBV3	4028	4239	0.43%	0.047%
85	26.414	3985	3987	3988	rBV2	4078	2699	0.27%	0.030%
86	26.984	4076	4084	4085	rBV7	13323	26169	2.67%	0.287%
87	27.753	4213	4215	4216	rVB	4993	2658	0.27%	0.029%
88	27.959	4249	4250	4252	rVB2	5363	2517	0.26%	0.028%
89	28.423	4325	4329	4334	rBV8	4565	8540	0.87%	0.094%
90	28.852	4400	4402	4404	rBV3	4276	3272	0.33%	0.036%
91	29.158	4452	4454	4457	rBV4	4303	4098	0.42%	0.045%
92	29.187	4457	4459	4460	rVV2	3880	1799	0.18%	0.020%
93	29.205	4460	4462	4465	rVB4	3485	1989	0.20%	0.022%
94	29.634	4534	4535	4536	rVB	4729	1669	0.17%	0.018%
95	29.692	4543	4545	4546	rBV2	5588	3465	0.35%	0.038%
96	30.092	4612	4613	4616	rVB3	7070	3989	0.41%	0.044%
97	30.515	4683	4685	4687	rBV3	3876	2648	0.27%	0.029%
98	30.856	4741	4743	4745	rBV3	3822	3639	0.37%	0.040%
99	30.973	4761	4763	4765	rBV3	3596	3401	0.35%	0.037%
100	31.807	4903	4905	4907	rBV3	5205	5581	0.57%	0.061%


Sum of corrected areas: 9111240

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
Data File : BG061538.D
Acq On : 7 Jun 2024 18:16
Operator : MA/JU
Sample : PB161251BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

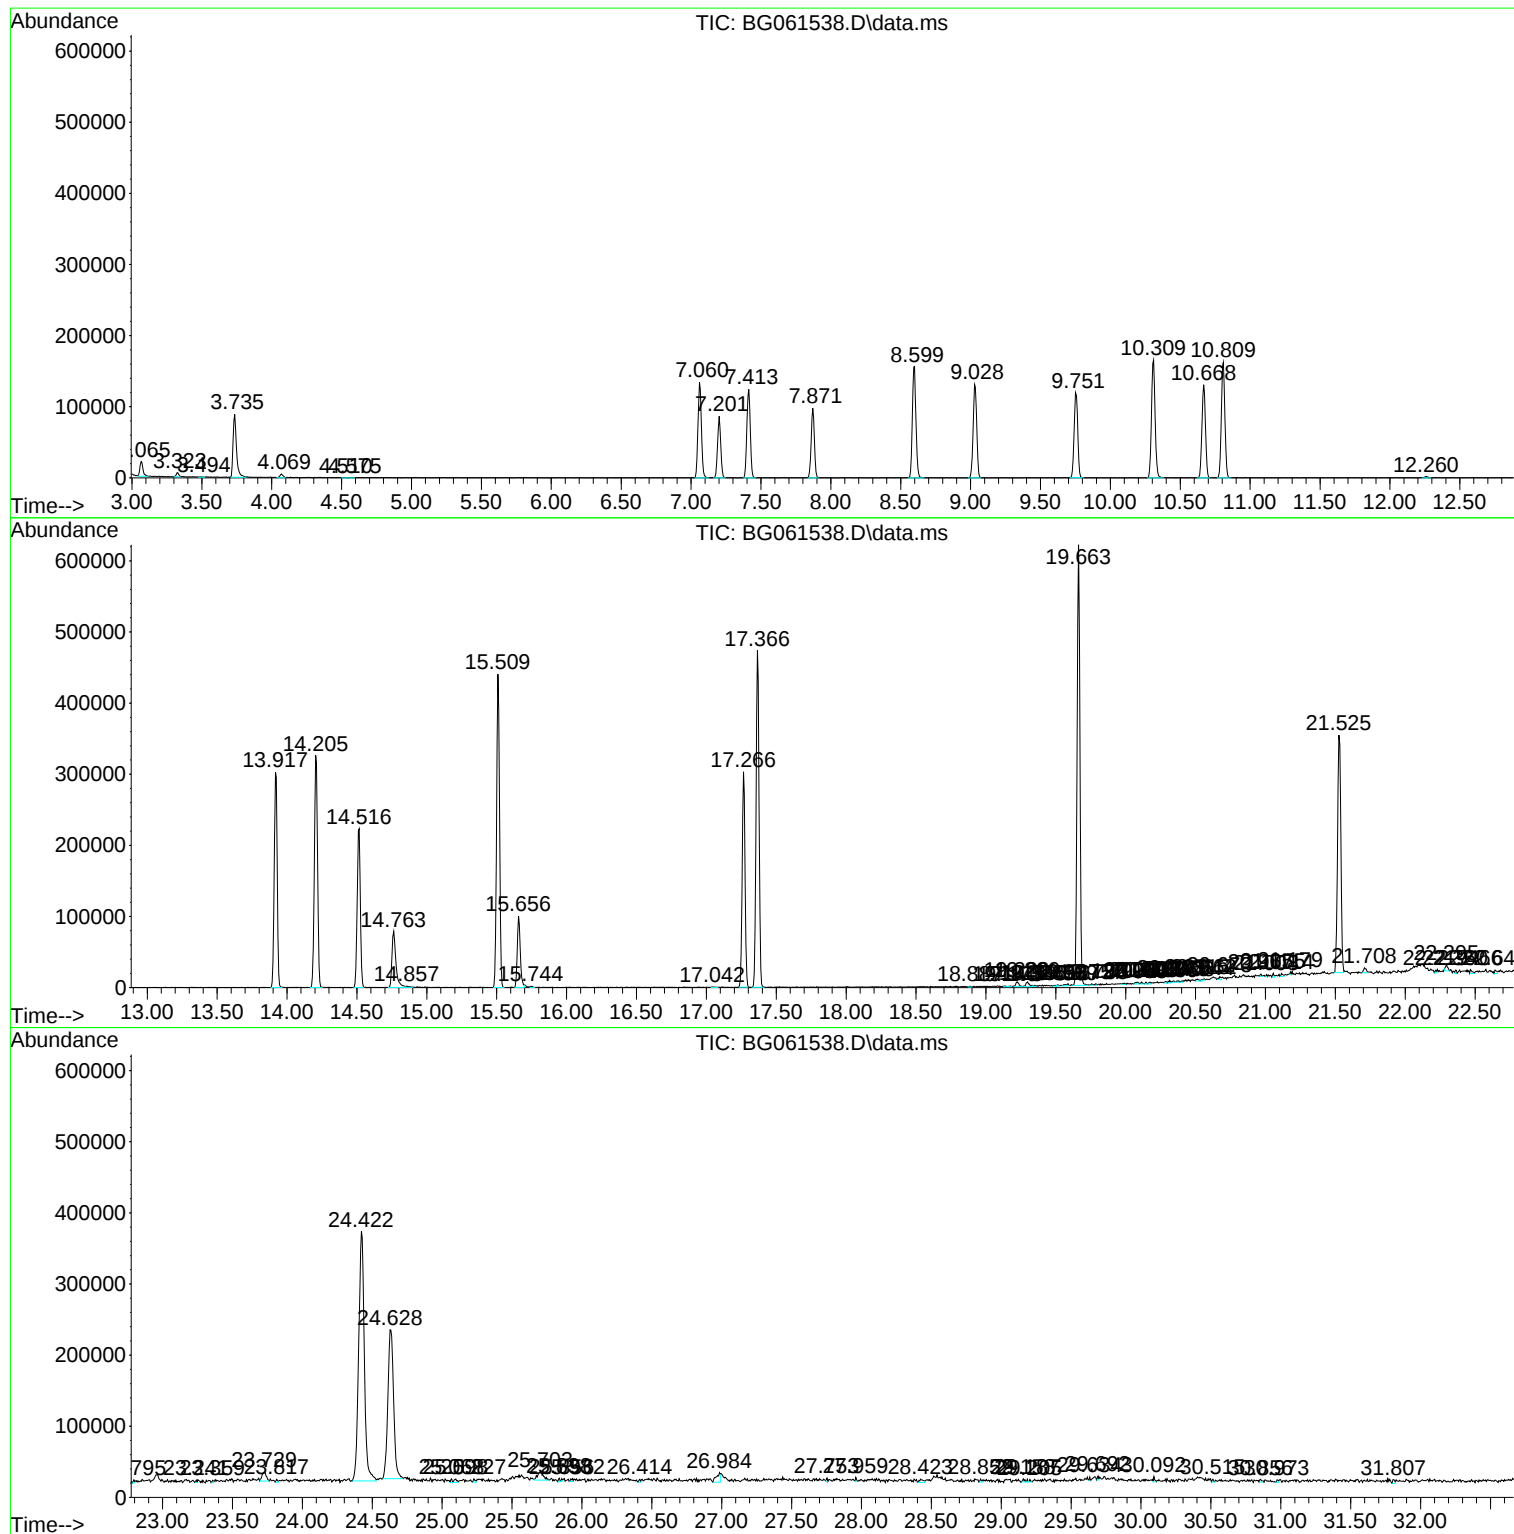

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
Data File : BG061538.D
Acq On : 7 Jun 2024 18:16
Operator : MA/JU
Sample : PB161251BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK251










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.065	4.01 ng/ul	31574	1,4-Dichlorobenzene-d4	7.871

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	42		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	42		
3	2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25		
4	3,4-Hexanediol, 2,5-dimethyl-	146	C8H18O2	022607-11-0	23		
5	3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23		

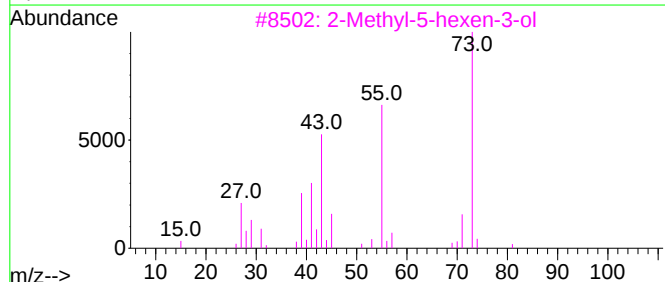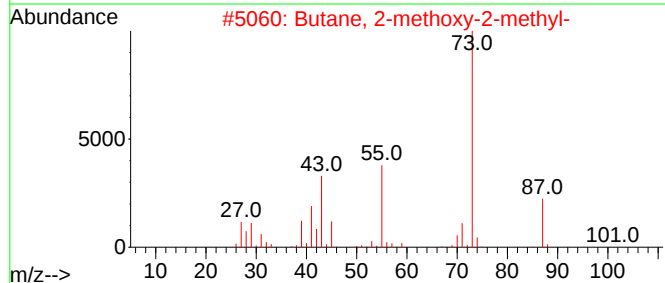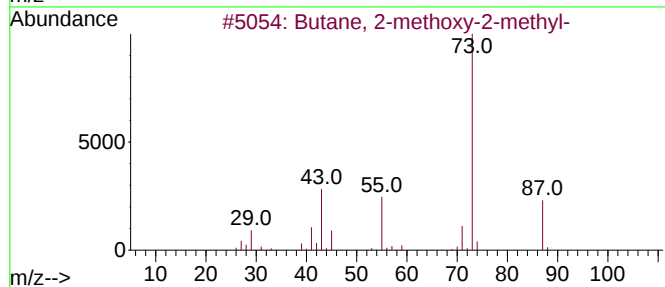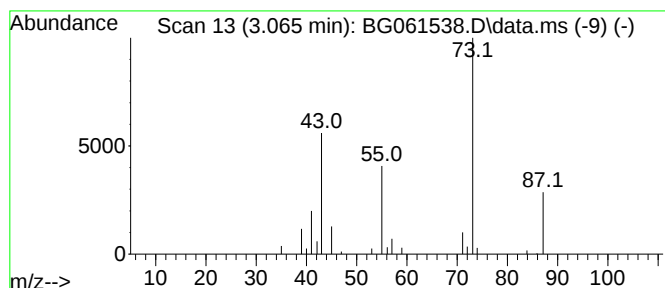

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060724\
Data File : BG061538.D
Acq On : 7 Jun 2024 18:16
Operator : MA/JU
Sample : PB161251BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.065	4.0	ng/u1	31574	1	7.871	157444	20.0