

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060819\
 Data File : BG041150.D
 Acq On : 9 Jun 2019 2:54
 Operator : HP/JU
 Sample : 8270PBBL2
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 8270PBBL2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.640	427	434	450	rBV	756523	1202386	30.01%	6.832%
2	7.250	700	708	719	rBV	813309	1415783	35.34%	8.045%
3	7.632	765	773	786	rBV	765101	1338932	33.42%	7.608%
4	8.102	847	853	861	rBV	124868	223556	5.58%	1.270%
5	8.425	901	908	918	rVB	568027	974889	24.33%	5.540%
6	9.283	1046	1054	1065	rBV	492681	892586	22.28%	5.072%
7	10.928	1325	1334	1346	rBV	178031	331679	8.28%	1.885%
8	13.361	1741	1748	1761	rBV	1461374	2278900	56.88%	12.950%
9	14.735	1976	1982	1996	rBV2	338970	538845	13.45%	3.062%
10	16.222	2228	2235	2250	rBV	1282372	1998685	49.89%	11.357%
11	17.479	2443	2449	2461	rVB	477579	727614	18.16%	4.135%
12	20.076	2885	2891	2901	rBV	3092696	4006308	100.00%	22.766%
13	21.757	3170	3177	3187	rBV	517622	861618	21.51%	4.896%
14	25.082	3733	3743	3756	rVB3	274559	806274	20.13%	4.582%


Sum of corrected areas: 17598055

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060819\
Data File : BG041150.D
Acq On : 9 Jun 2019 2:54
Operator : HP/JU
Sample : 8270PBBL2
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
8270PBBL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

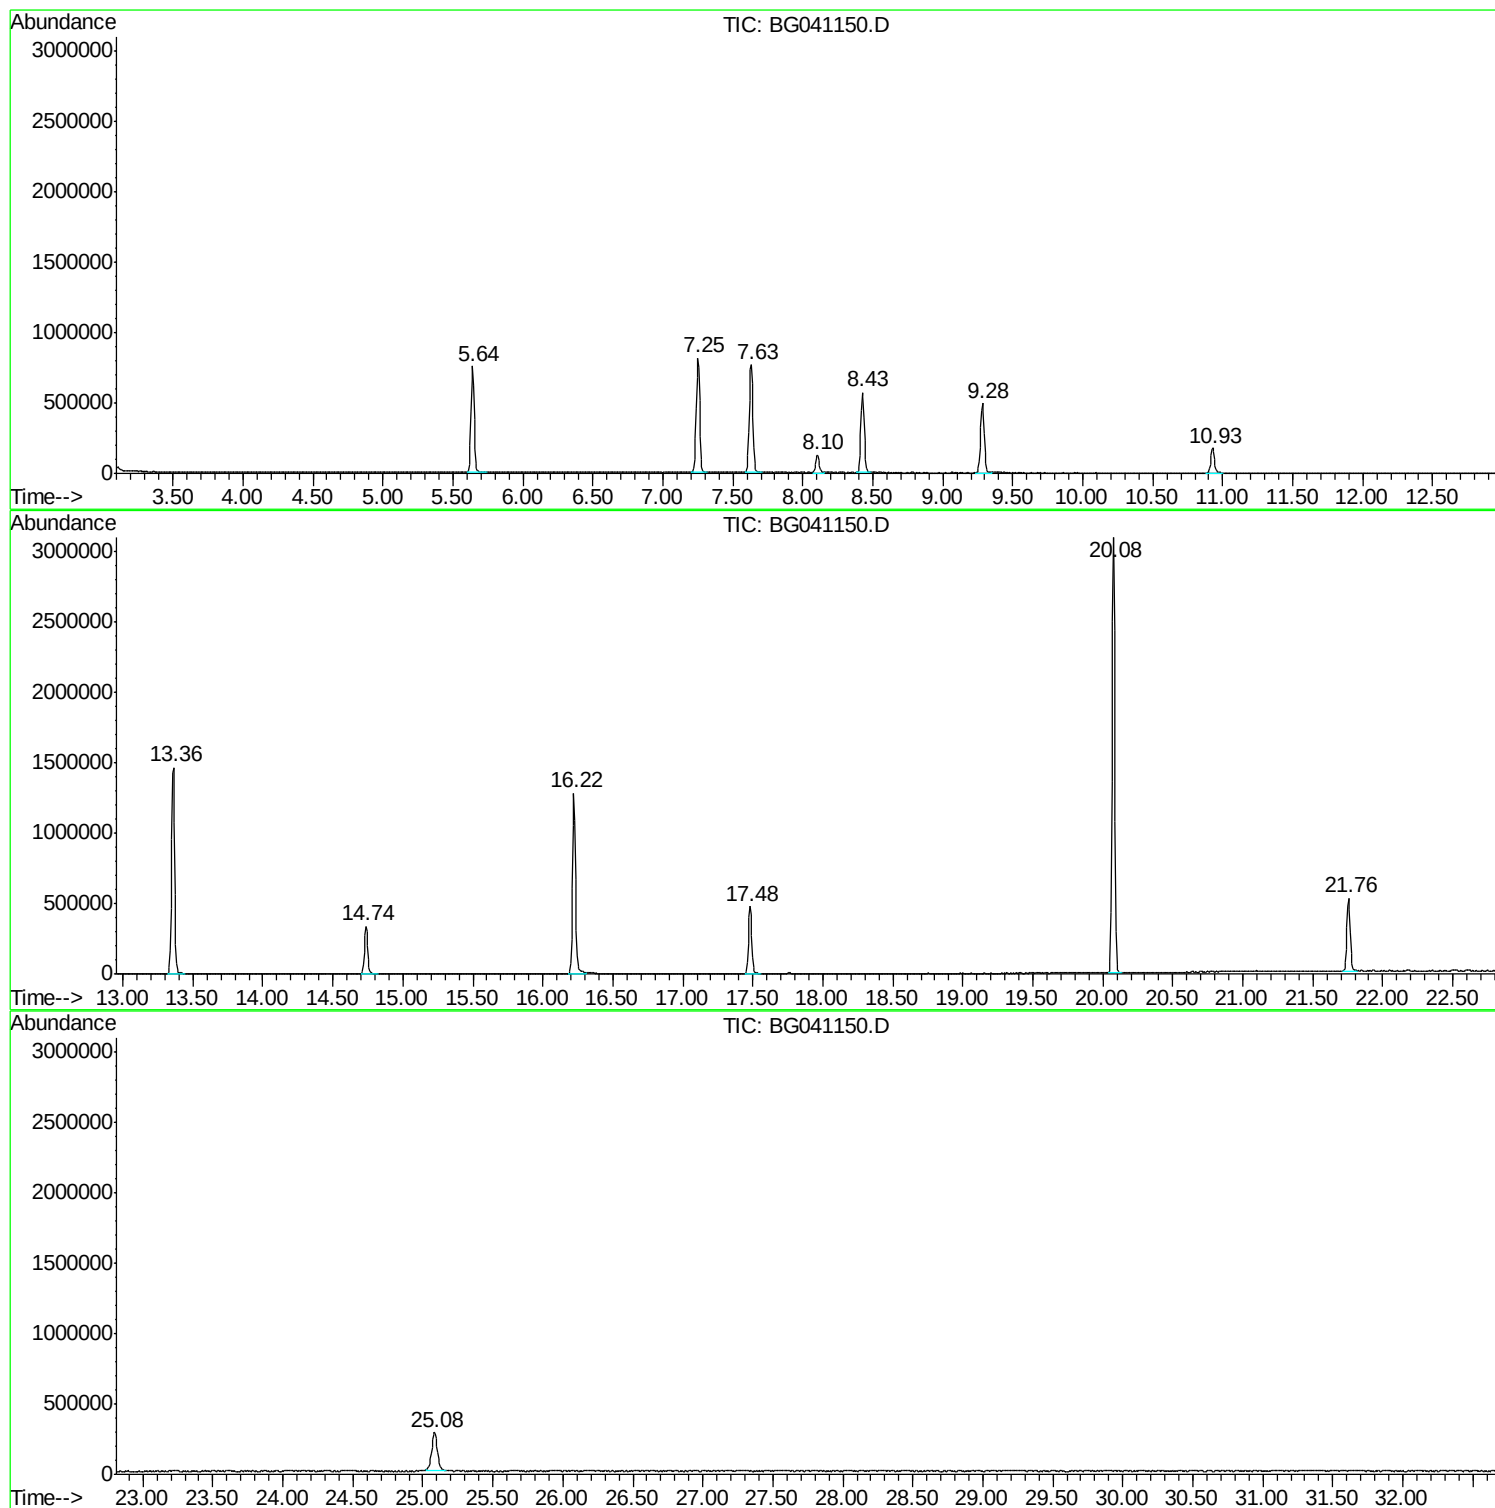

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060819\
Data_File : BG041150.D
Acq_On : 9-Jun-2019 2:544
Operator : HP/JUU
Sample : 8270PBBL2
Misc :
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
8270PBBL2

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
