


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060819\
 Data File : BG041127.D
 Acq On : 8 Jun 2019 11:04
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

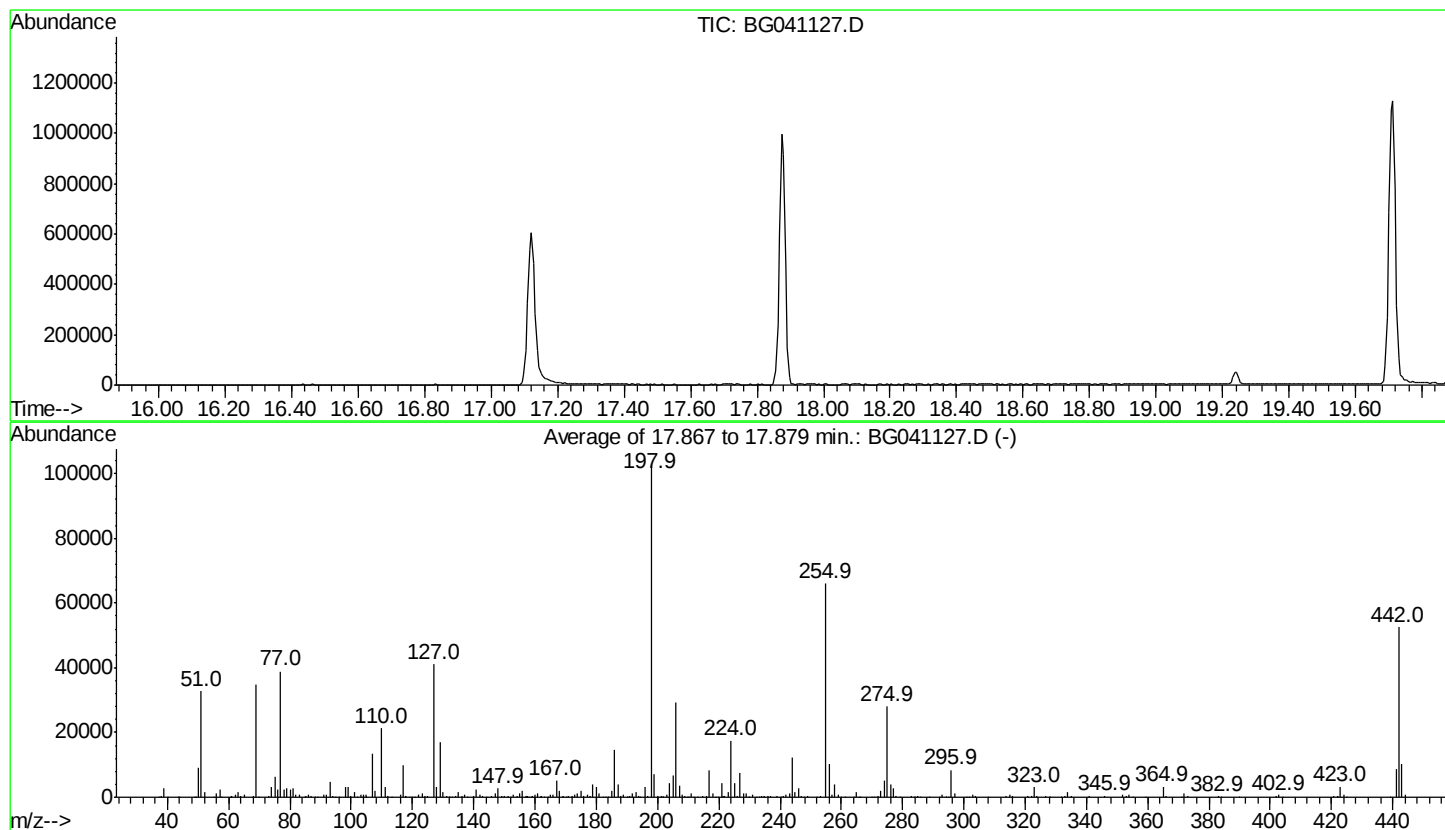

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	32661	PASS
68	69	0.00	2	0.7	259	PASS
69	198	0.00	100	34.0	34818	PASS
70	69	0.00	2	0.5	175	PASS
127	198	10	80	40.1	41141	PASS
197	198	0.00	2	0.4	368	PASS
198	198	100	100	100.0	102480	PASS
199	198	5	9	7.1	7261	PASS
275	198	10	60	27.3	27936	PASS
365	198	1	100	3.2	3239	PASS
441	198	0.01	100	8.6	8816	PASS
442	198	50	100	51.2	52493	PASS
443	442	15	24	19.8	10387	PASS