
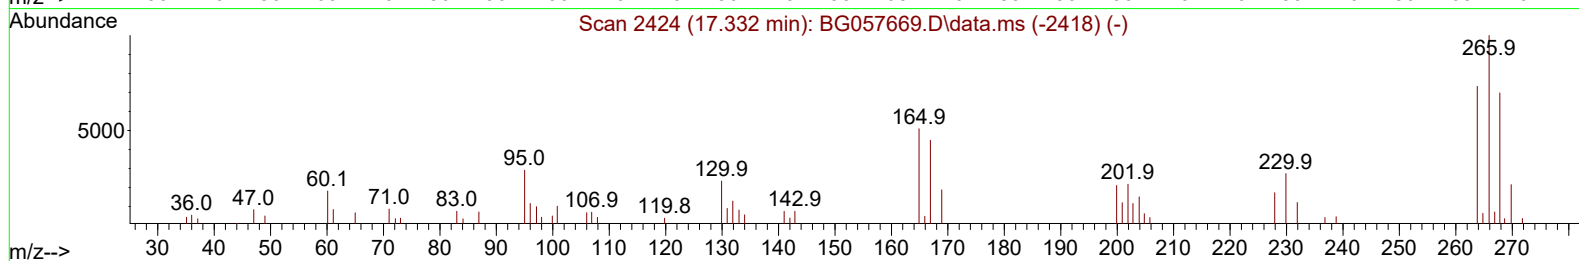
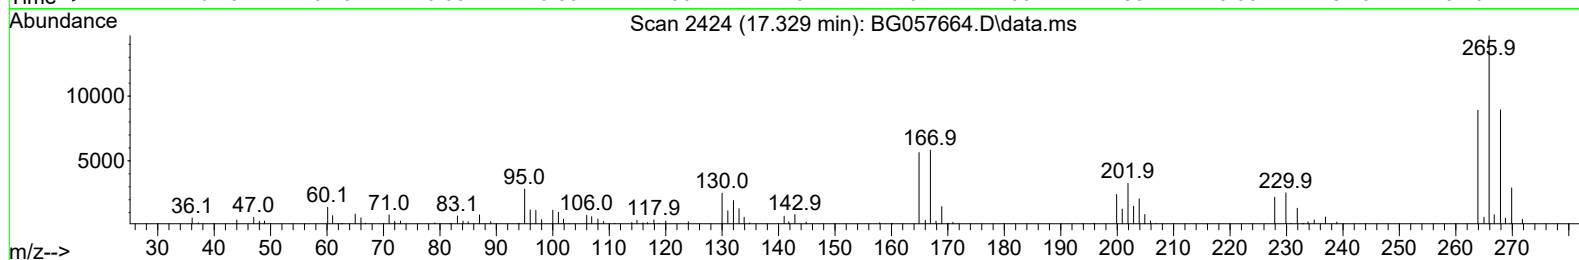


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060823\
Data File : BG057664.D
Acq On : 8 Jun 2023 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 05:34:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 00:44:37 2023
Response via : Initial Calibration

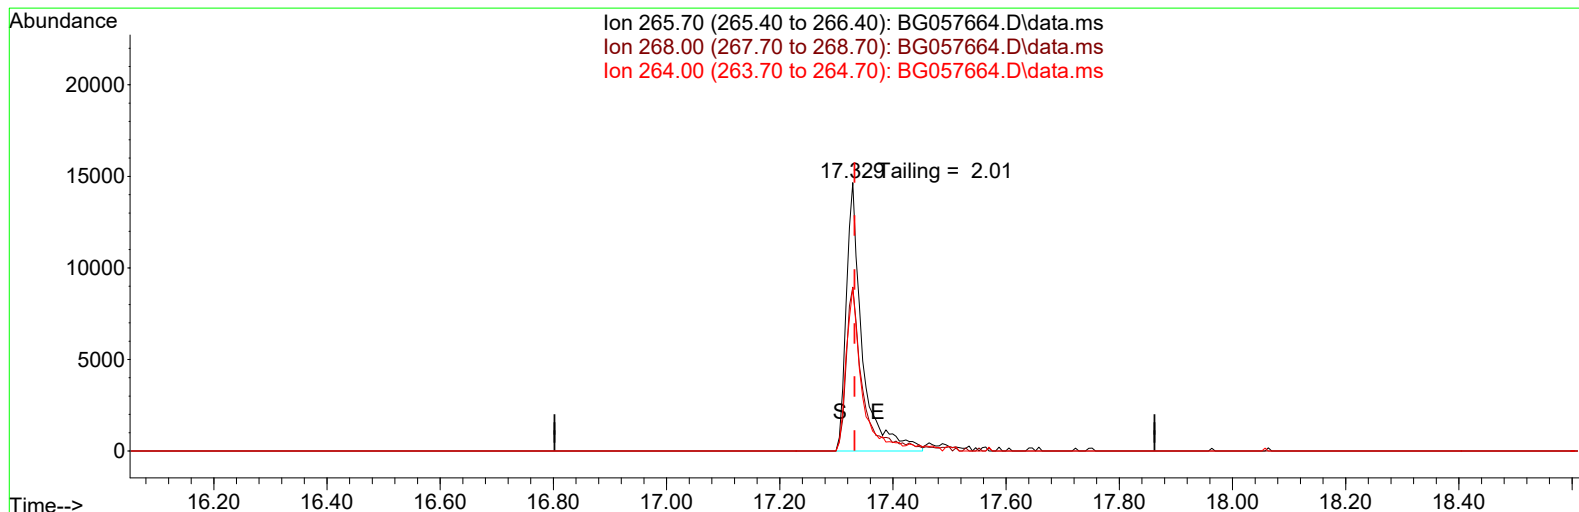

TIC: BG057664.D\data.ms

(70) Pentachlorophenol (C)




17.329min (-0.003) 19741.09 ng

response 28858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	73.40	61.05
264.00	73.20	60.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060823\
Data File : BG057664.D
Acq On : 8 Jun 2023 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 05:34:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 00:44:37 2023
Response via : Initial Calibration

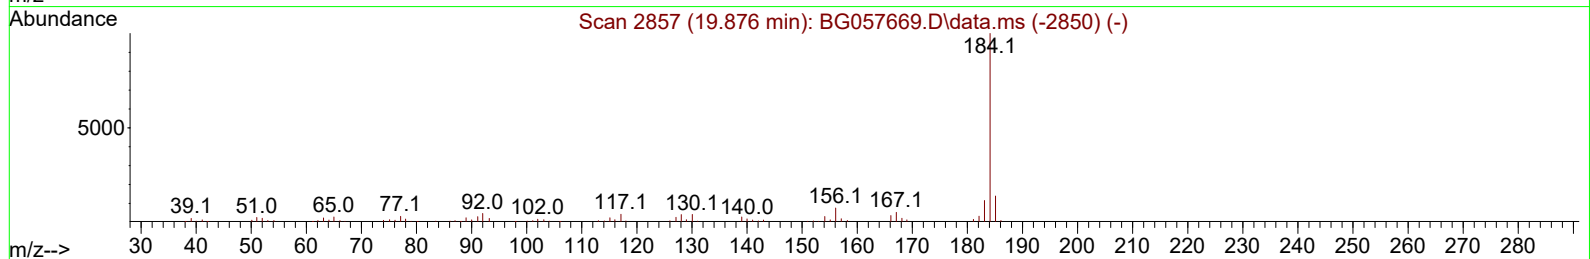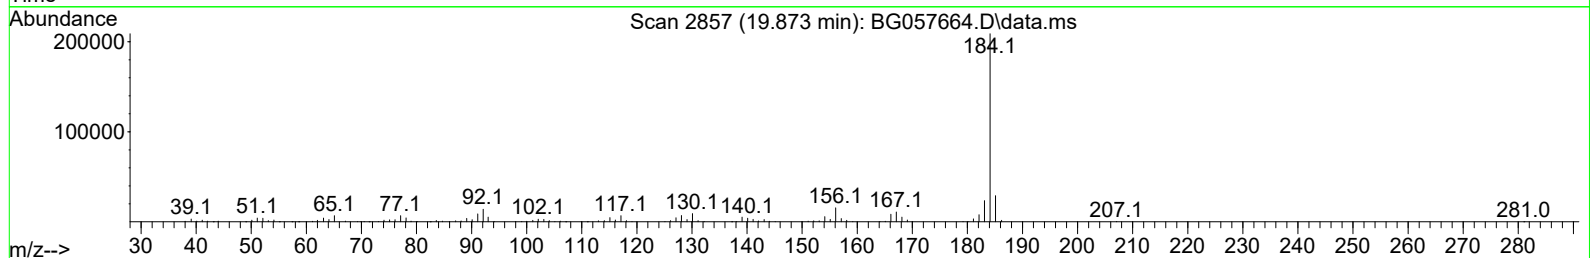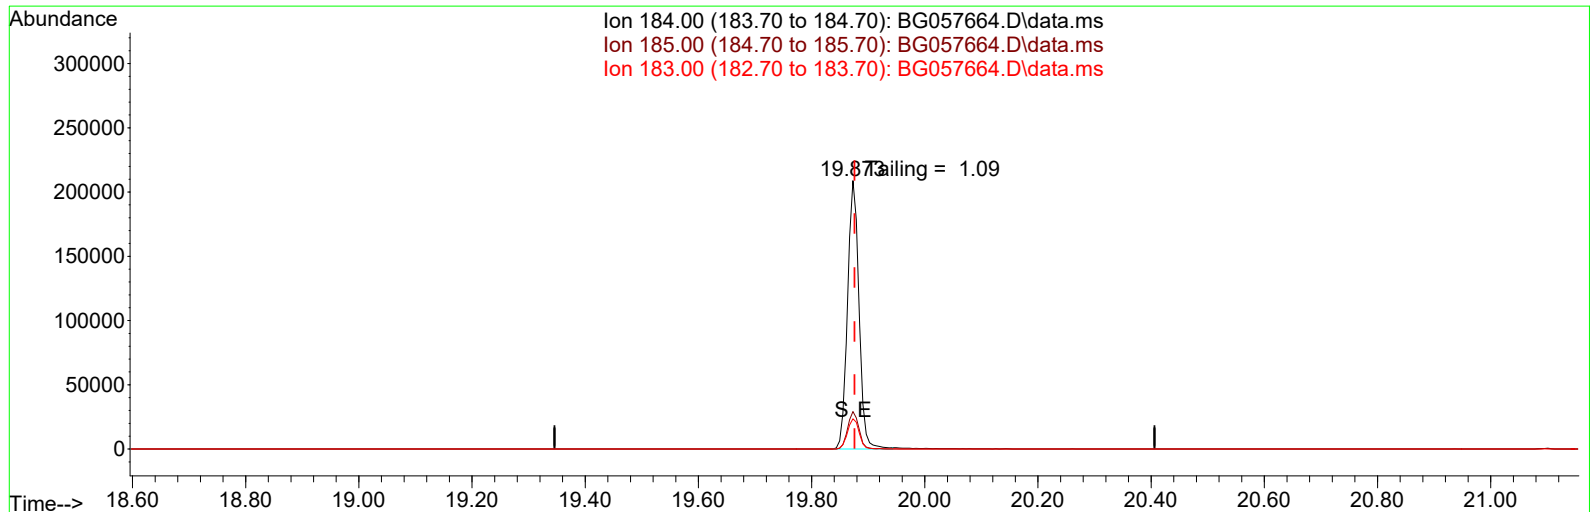

TIC: BG057664.D\data.ms

(77) Benzidine

19.873min (-0.003) 0.00 ng

response 294870

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.94
183.00	11.50	11.30
0.00	0.00	0.00