


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060823\
 Data File : BG057664.D
 Acq On : 8 Jun 2023 9:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 09 00:44:37 2023

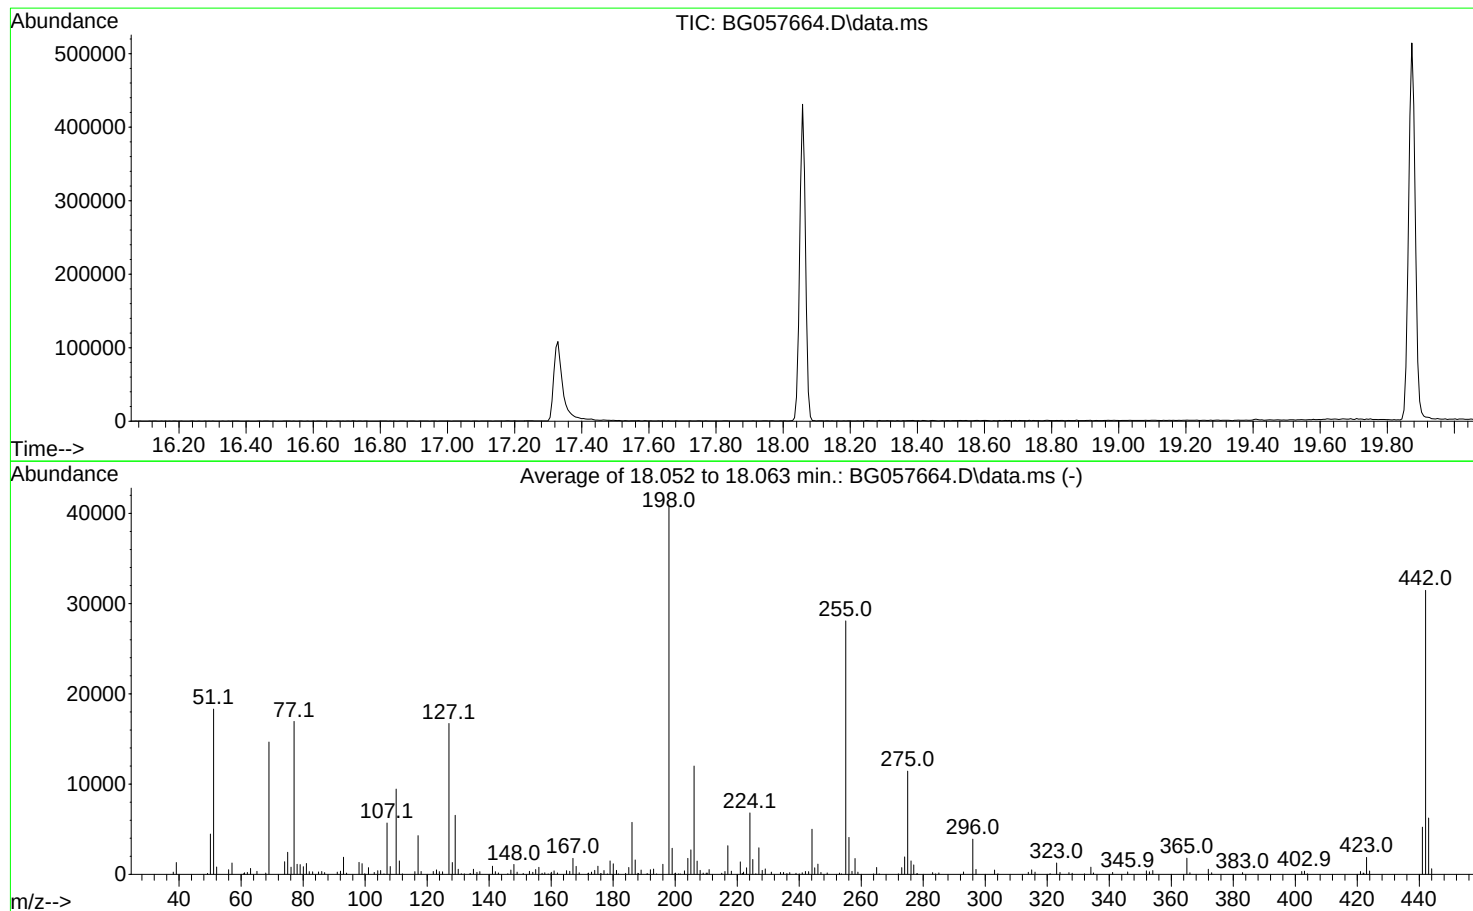

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	18319	PASS
68	69	0.00	2	1.0	147	PASS
69	198	0.00	100	36.0	14667	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	16717	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40763	PASS
199	198	5	9	7.1	2895	PASS
275	198	10	60	28.0	11432	PASS
365	198	1	100	4.4	1799	PASS
441	198	0.01	100	12.8	5226	PASS
442	442	50	100	100.0	31472	PASS
443	442	15	24	19.8	6241	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/8/2023	BNA_G	<u>BG057664.D</u>
Compound Name	Response	Retention Time
DDT	136255	21.095
DDD	1858	20.701
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1858	138113	1.35

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060823\
Data File : BG057664.D
Acq On : 8 Jun 2023 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 09 05:34:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 00:44:37 2023
Response via : Initial Calibration

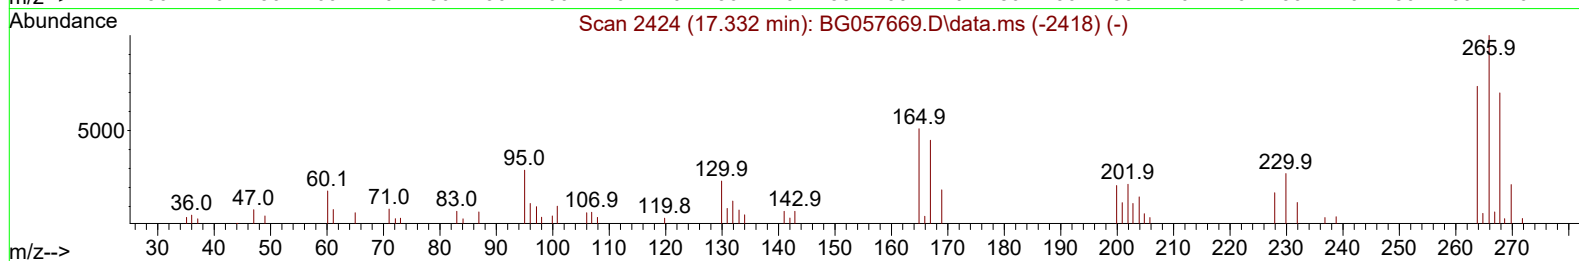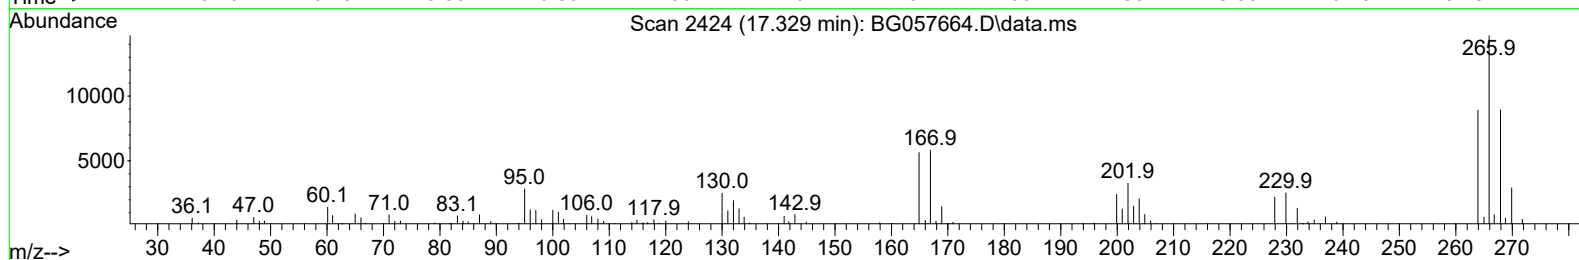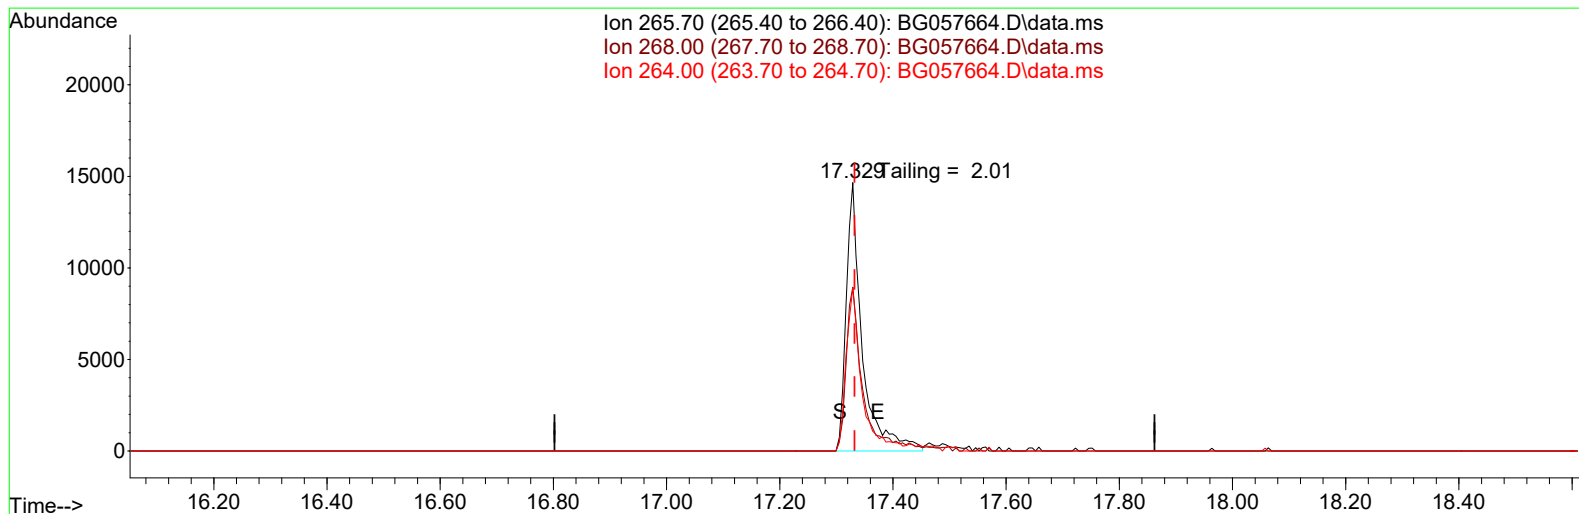

TIC: BG057664.D\data.ms

(70) Pentachlorophenol (C)

17.329min (-0.003) 19741.09 ng




response 28858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	73.40	61.05
264.00	73.20	60.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060823\
Data File : BG057664.D
Acq On : 8 Jun 2023 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 09 05:34:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 00:44:37 2023
Response via : Initial Calibration

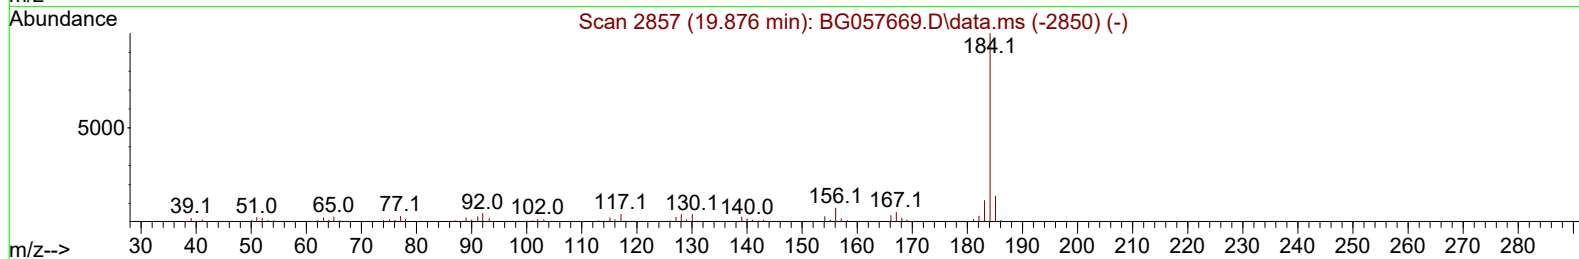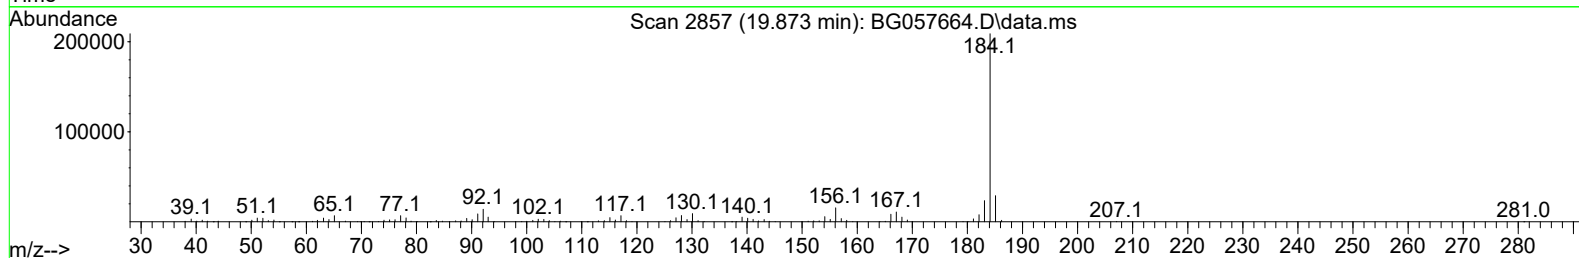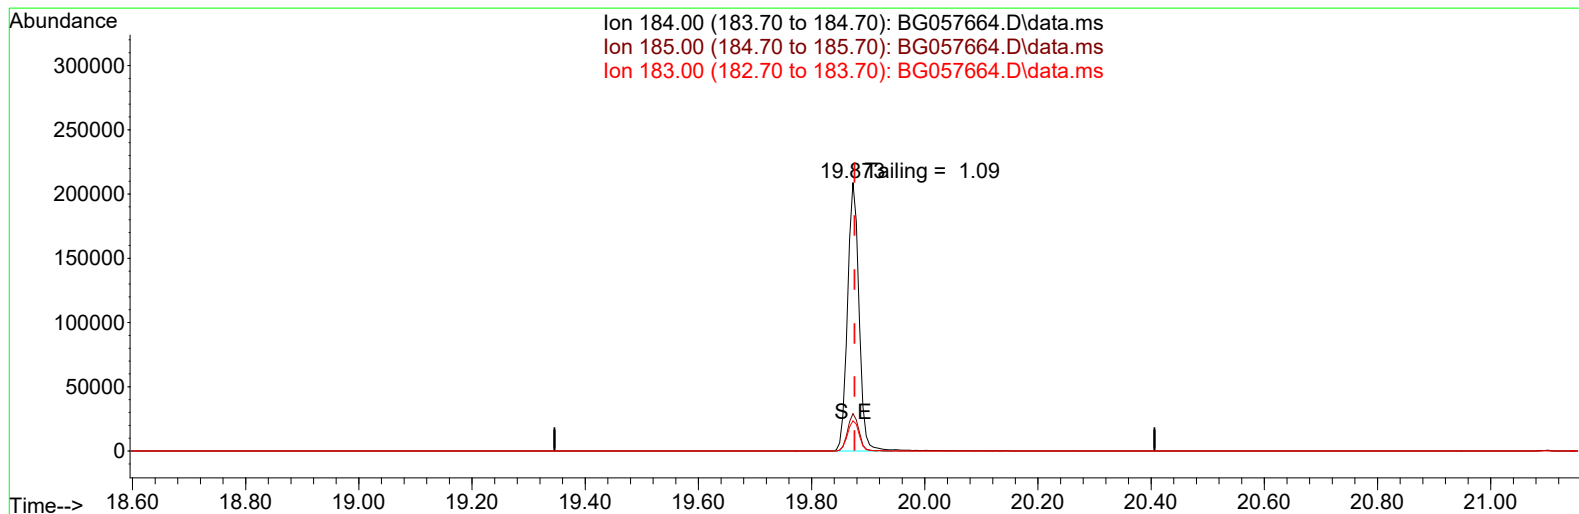

TIC: BG057664.D\data.ms

(77) Benzidine

19.873min (-0.003) 0.00 ng

response 294870

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.94
183.00	11.50	11.30
0.00	0.00	0.00