

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061019\
 Data File : BG041157.D
 Acq On : 10 Jun 2019 9:46
 Operator : HP/JU
 Sample : PB120413BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120413BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.641	427	434	446	rBV	637322	1013634	34.06%	6.551%
2	7.251	698	708	717	rBV	716928	1222839	41.09%	7.903%
3	7.633	765	773	786	rBV	652550	1136559	38.19%	7.345%
4	8.103	846	853	861	rBV	167996	287851	9.67%	1.860%
5	8.426	900	908	918	rBV	472331	824697	27.71%	5.330%
6	9.284	1046	1054	1062	rBV	416746	752306	25.28%	4.862%
7	10.929	1326	1334	1345	rBV	233475	443078	14.89%	2.863%
8	13.361	1741	1748	1761	rBV	1245722	1960768	65.89%	12.671%
9	14.736	1976	1982	1997	rBV2	419621	684124	22.99%	4.421%
10	16.223	2228	2235	2249	rBV	919036	1459937	49.06%	9.435%
11	17.480	2442	2449	2464	rBV2	553663	855514	28.75%	5.529%
12	20.077	2884	2891	2898	rBV	2311234	2975940	100.00%	19.232%
13	21.757	3170	3177	3186	rBV2	563615	958322	32.20%	6.193%
14	25.083	3731	3743	3756	rBV	291262	898462	30.19%	5.806%


Sum of corrected areas: 15474031

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061019\
Data File : BG041157.D
Acq On : 10 Jun 2019 9:46
Operator : HP/JU
Sample : PB120413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120413BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

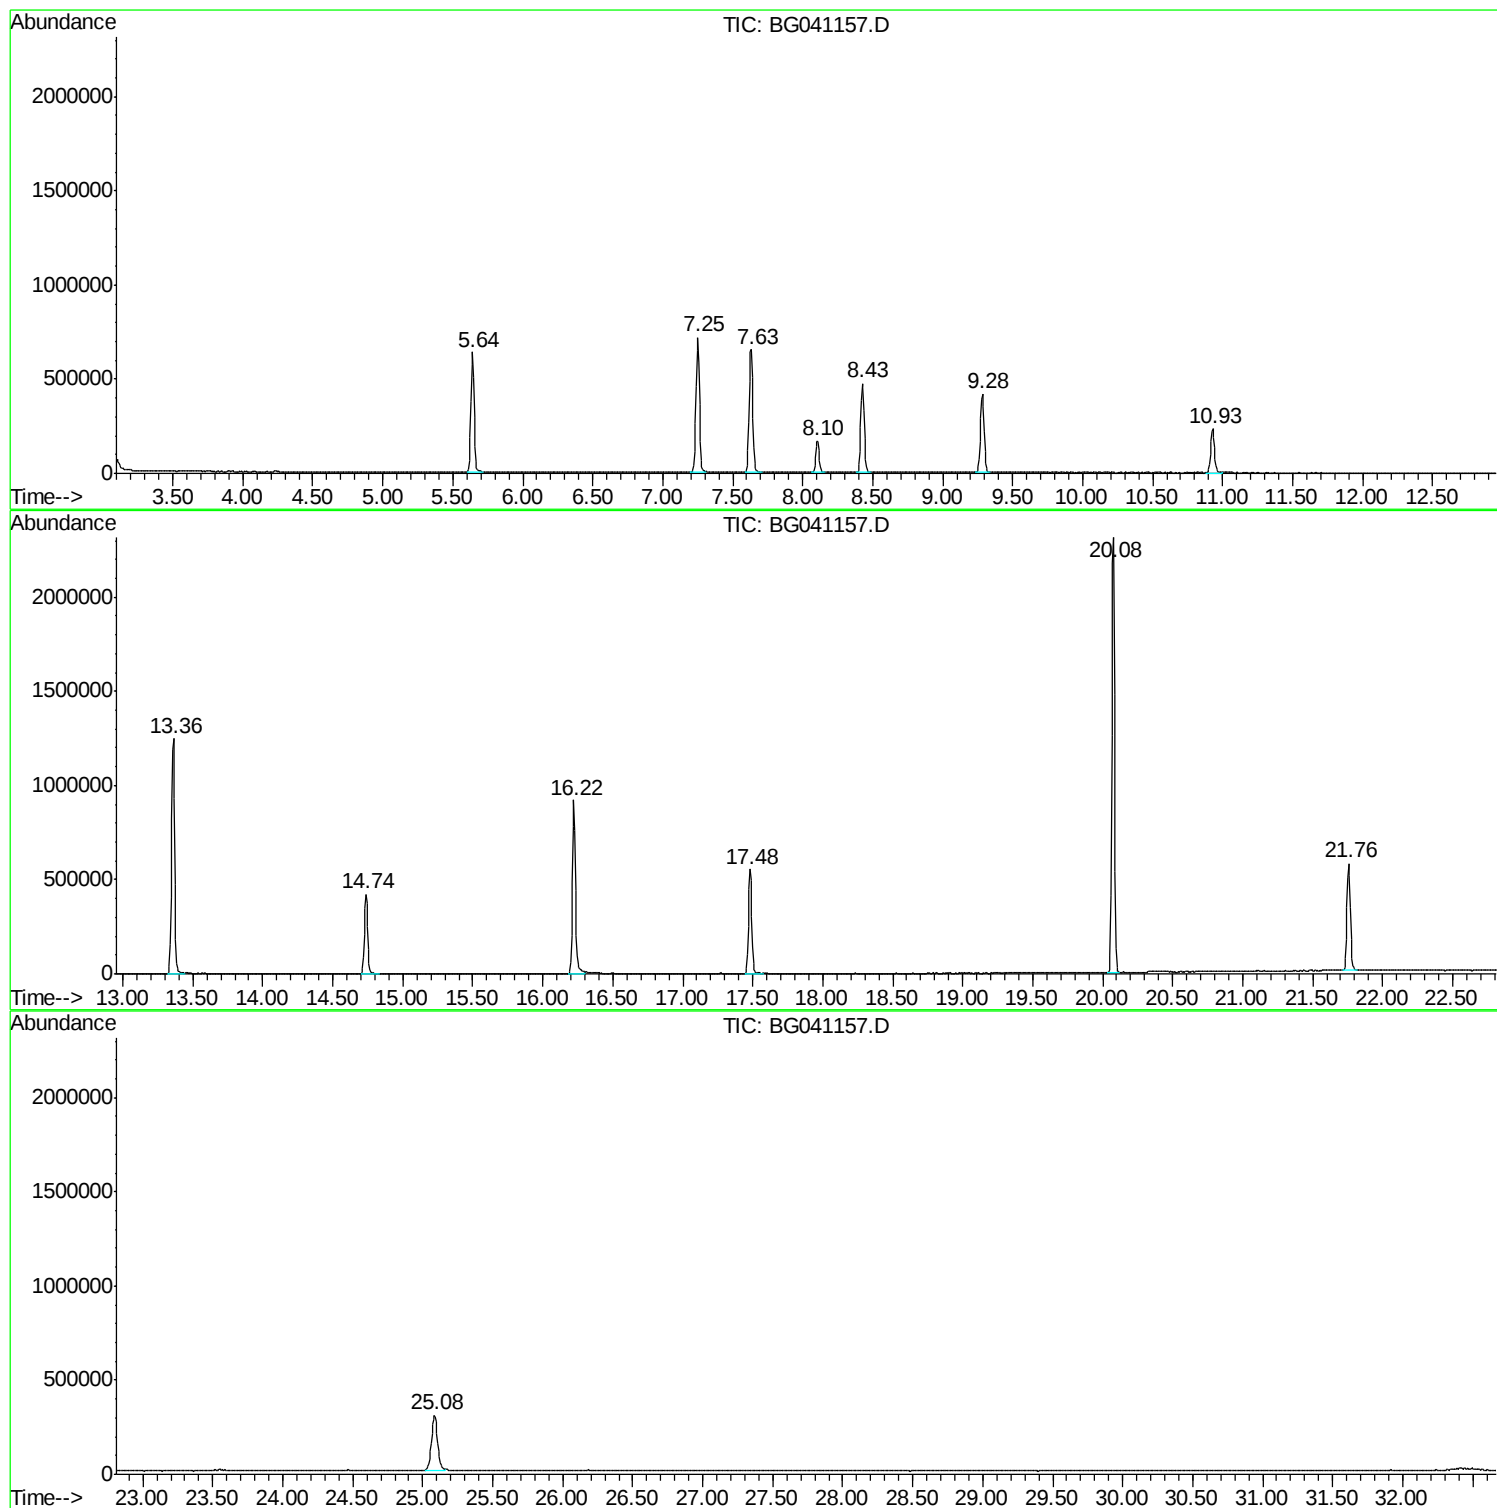

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061019\
Data File : BG041157.D
Acq On : 10 Jun 2019 9:46
Operator : HP/JU
Sample : PB120413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120413BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.63	78.97 ng	1136560	1,4-Dichlorobenzene-d4	8.11

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

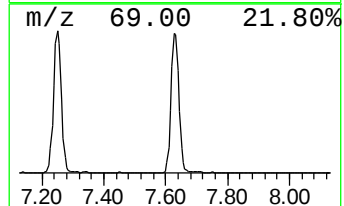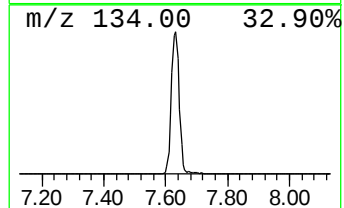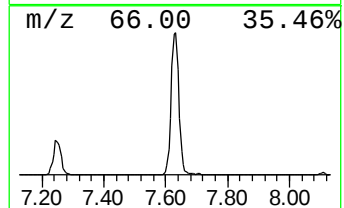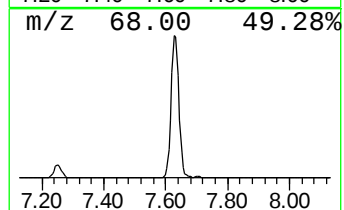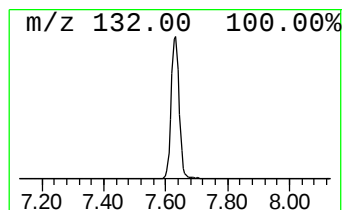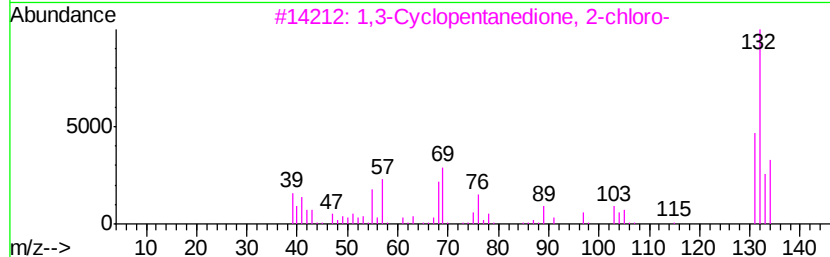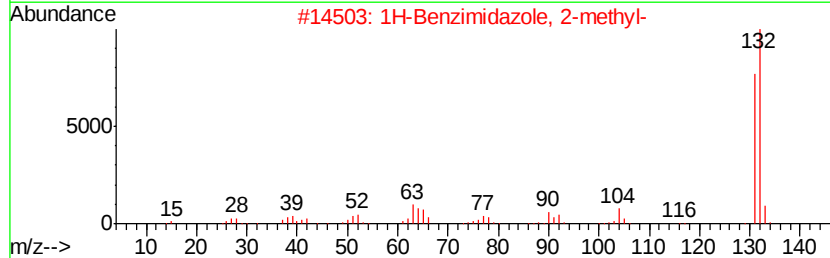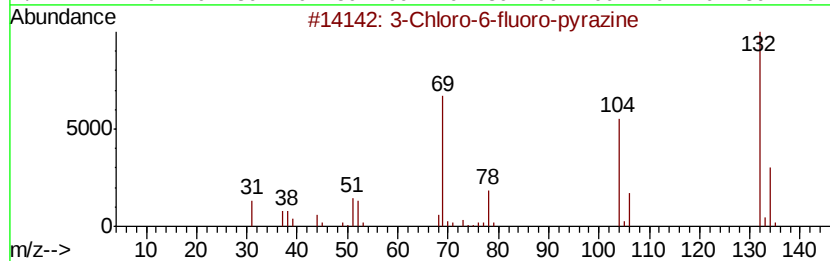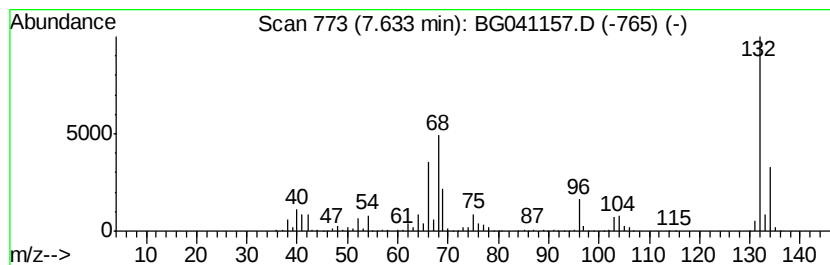

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061019\
Data File : BG041157.D
Acq On : 10 Jun 2019 9:46
Operator : HP/JU
Sample : PB120413BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120413BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.63	7.63	79.0	ng	1136560	1	8.11	287851	20.0