


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061019\
 Data File : BG041155.D
 Acq On : 10 Jun 2019 8:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

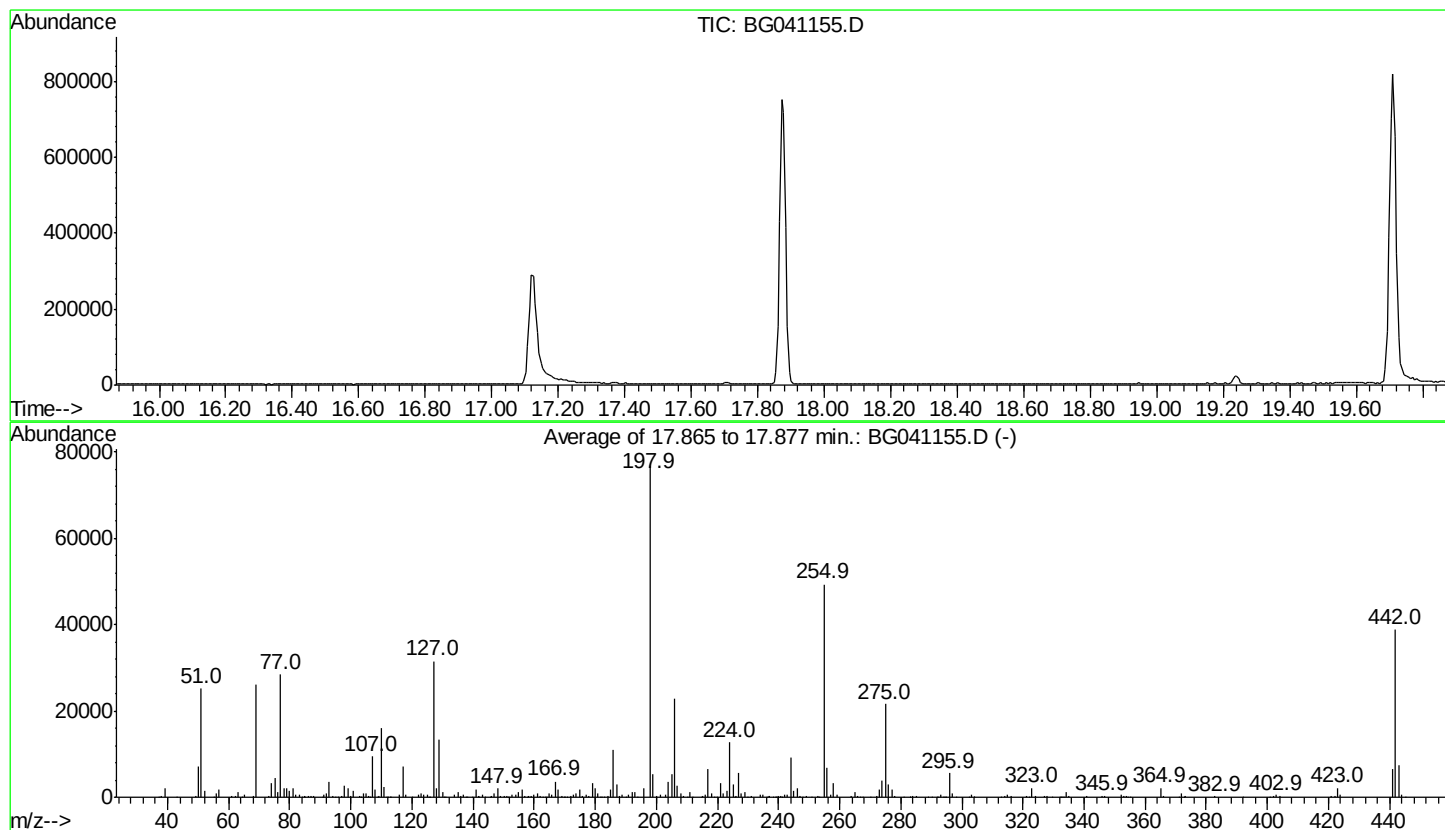

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	25194	PASS
68	69	0.00	2	1.2	314	PASS
69	198	0.00	100	34.1	26194	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	31517	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76778	PASS
199	198	5	9	7.1	5467	PASS
275	198	10	60	28.1	21578	PASS
365	198	1	100	2.8	2134	PASS
441	198	0.01	100	8.5	6534	PASS
442	198	50	100	50.4	38690	PASS
443	442	15	24	19.3	7463	PASS