


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061019\
 Data File : BG041164.D
 Acq On : 10 Jun 2019 15:44
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

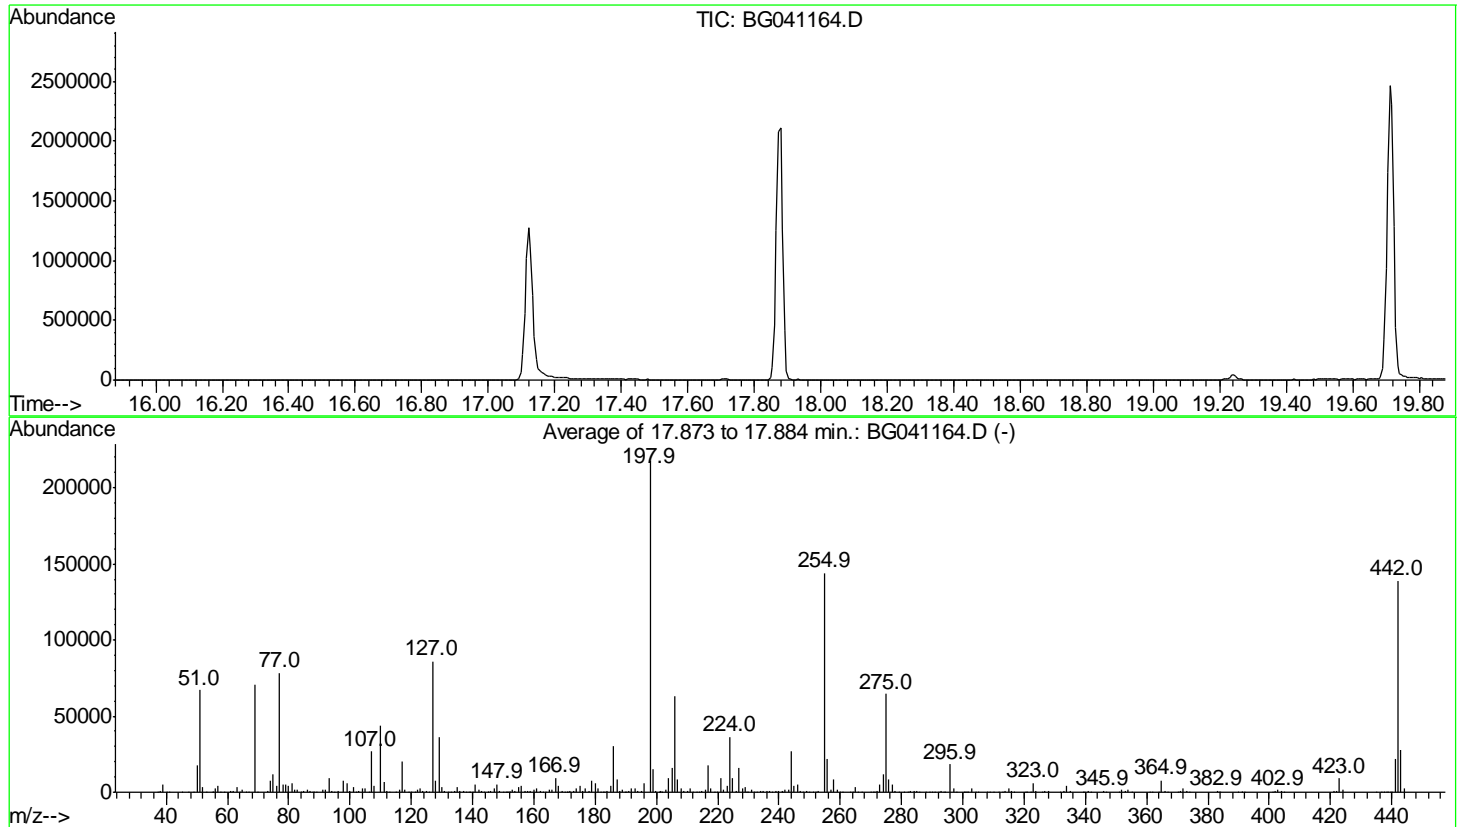

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	67037	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	70944	PASS
70	69	0.00	2	0.5	351	PASS
127	198	10	80	39.5	85976	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	217877	PASS
199	198	5	9	7.1	15478	PASS
275	198	10	60	29.6	64541	PASS
365	198	1	100	3.5	7711	PASS
441	198	0.01	100	9.9	21581	PASS
442	198	50	100	63.7	138896	PASS
443	442	15	24	19.8	27450	PASS