

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061119\
 Data File : BG041182.D
 Acq On : 11 Jun 2019 10:22
 Operator : HP/JU
 Sample : PB120476BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB120476BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.643	428	435	448	rBV	829179	1373706	34.24%	7.241%
2	7.259	701	710	724	rBV	907303	1646535	41.04%	8.679%
3	7.635	766	774	783	rBV	893303	1551828	38.68%	8.179%
4	8.105	847	854	863	rBV	152693	260328	6.49%	1.372%
5	8.428	902	909	919	rBV	655463	1125624	28.06%	5.933%
6	9.286	1046	1055	1066	rBV	574998	1054612	26.29%	5.559%
7	10.925	1327	1334	1345	rBV	199201	376982	9.40%	1.987%
8	13.358	1741	1748	1764	rBV	1654115	2685810	66.95%	14.156%
9	14.739	1975	1983	1994	rBV2	356158	591053	14.73%	3.115%
10	16.225	2227	2236	2254	rBV	1330598	2138404	53.30%	11.271%
11	17.482	2443	2450	2464	rBV	476523	729704	18.19%	3.846%
12	20.079	2885	2892	2903	rBV	2880822	4011859	100.00%	21.146%
13	21.760	3171	3178	3191	rBV2	438286	796065	19.84%	4.196%
14	25.091	3733	3745	3755	rBV	187752	629921	15.70%	3.320%


Sum of corrected areas: 18972431

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061119\
Data File : BG041182.D
Acq On : 11 Jun 2019 10:22
Operator : HP/JU
Sample : PB120476BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120476BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

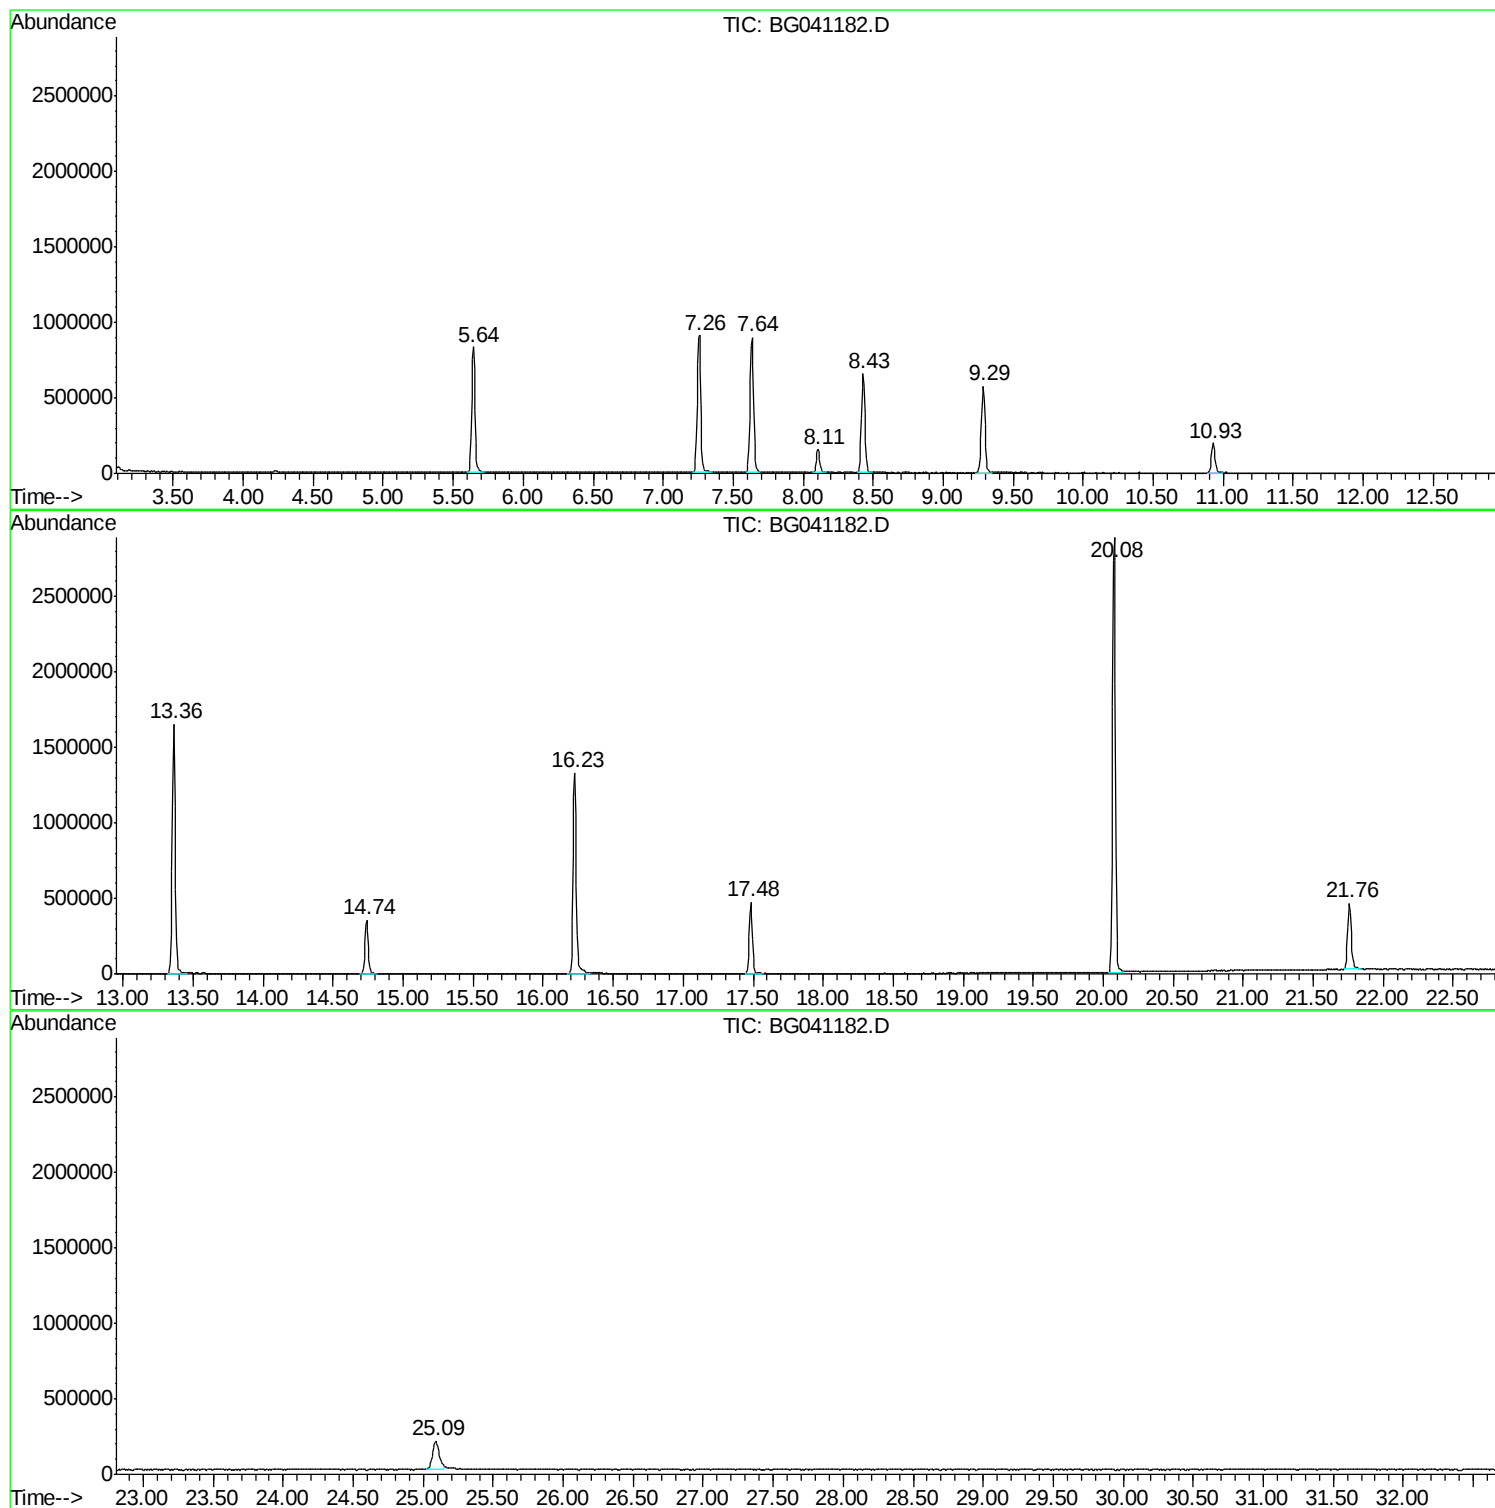

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061119\
Data File : BG041182.D
Acq On : 11 Jun 2019 10:22
Operator : HP/JU
Sample : PB120476BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120476BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.64 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.64	119.22 ng	1551830	1,4-Dichlorobenzene-d4	8.11

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	22
3		5-Aminoindole	132	C8H8N2	005192-03-0	22
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16

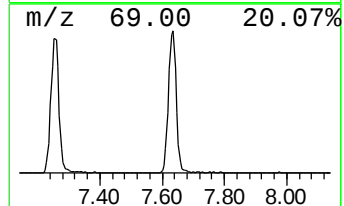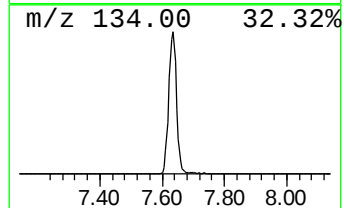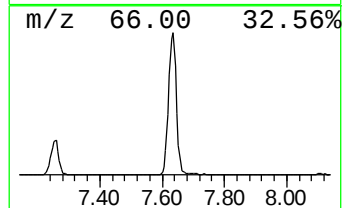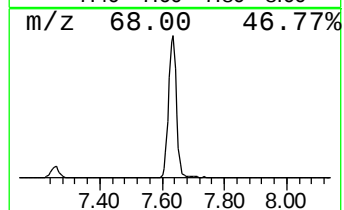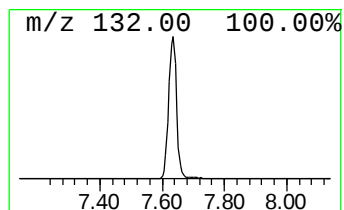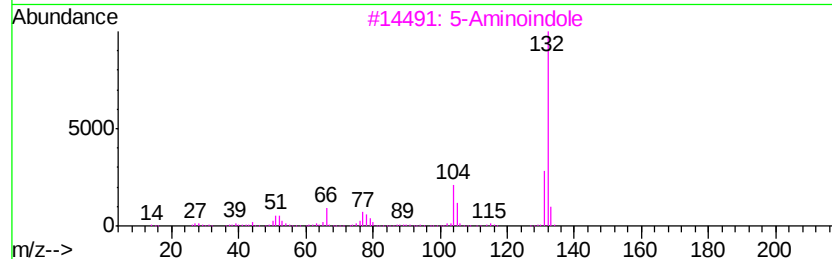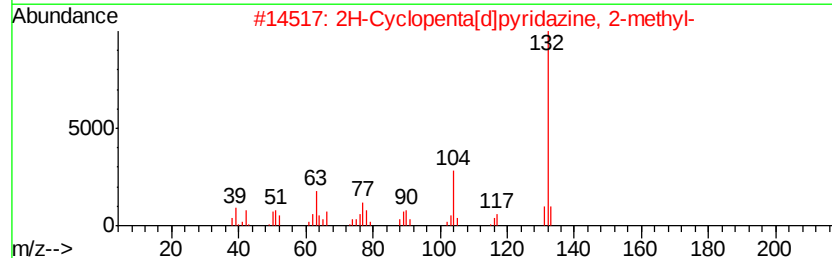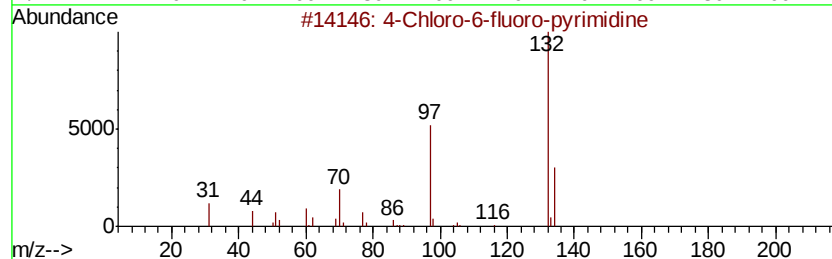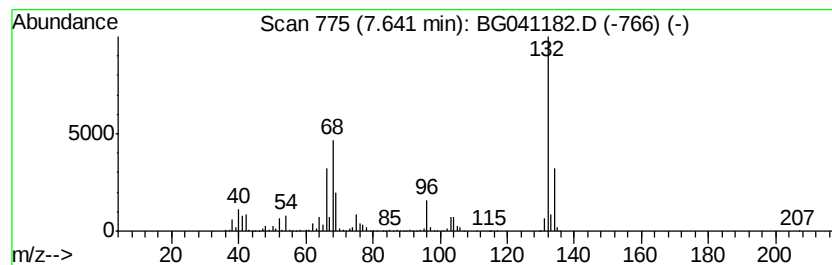

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061119\
Data File : BG041182.D
Acq On : 11 Jun 2019 10:22
Operator : HP/JU
Sample : PB120476BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB120476BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.64	7.64	119.2	ng	1551830	1	8.11	260328	20.0