


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG061119\
 Data File : BG041179.D
 Acq On : 11 Jun 2019 7:47
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

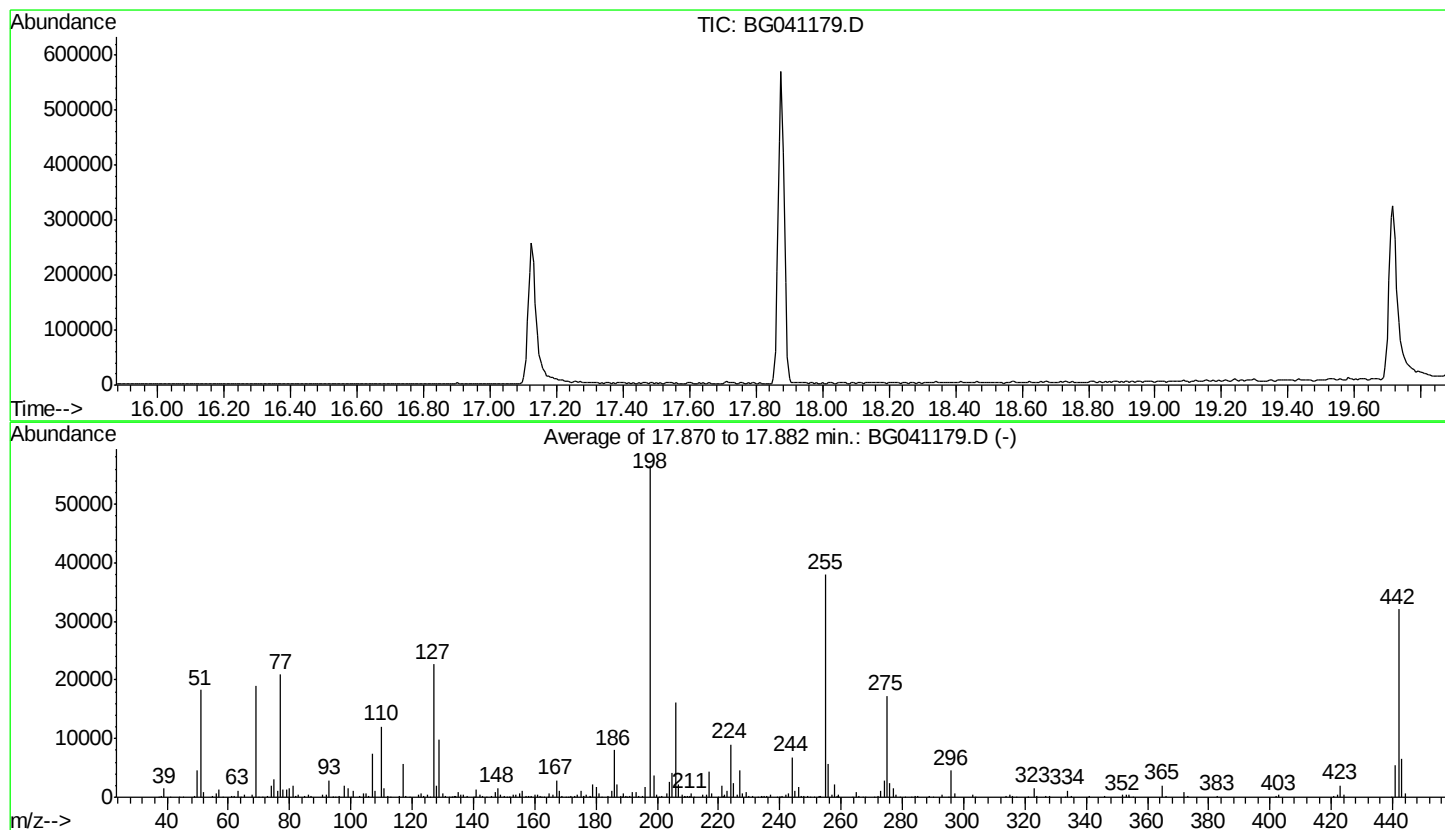

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	18294	PASS
68	69	0.00	2	2.0	386	PASS
69	198	0.00	100	33.6	19007	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	40.1	22712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56573	PASS
199	198	5	9	6.5	3656	PASS
275	198	10	60	30.6	17298	PASS
365	198	1	100	3.6	2032	PASS
441	198	0.01	100	9.6	5412	PASS
442	198	50	100	56.6	32026	PASS
443	442	15	24	20.3	6505	PASS