


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061119\
 Data File : BG041193.D
 Acq On : 11 Jun 2019 17:22
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

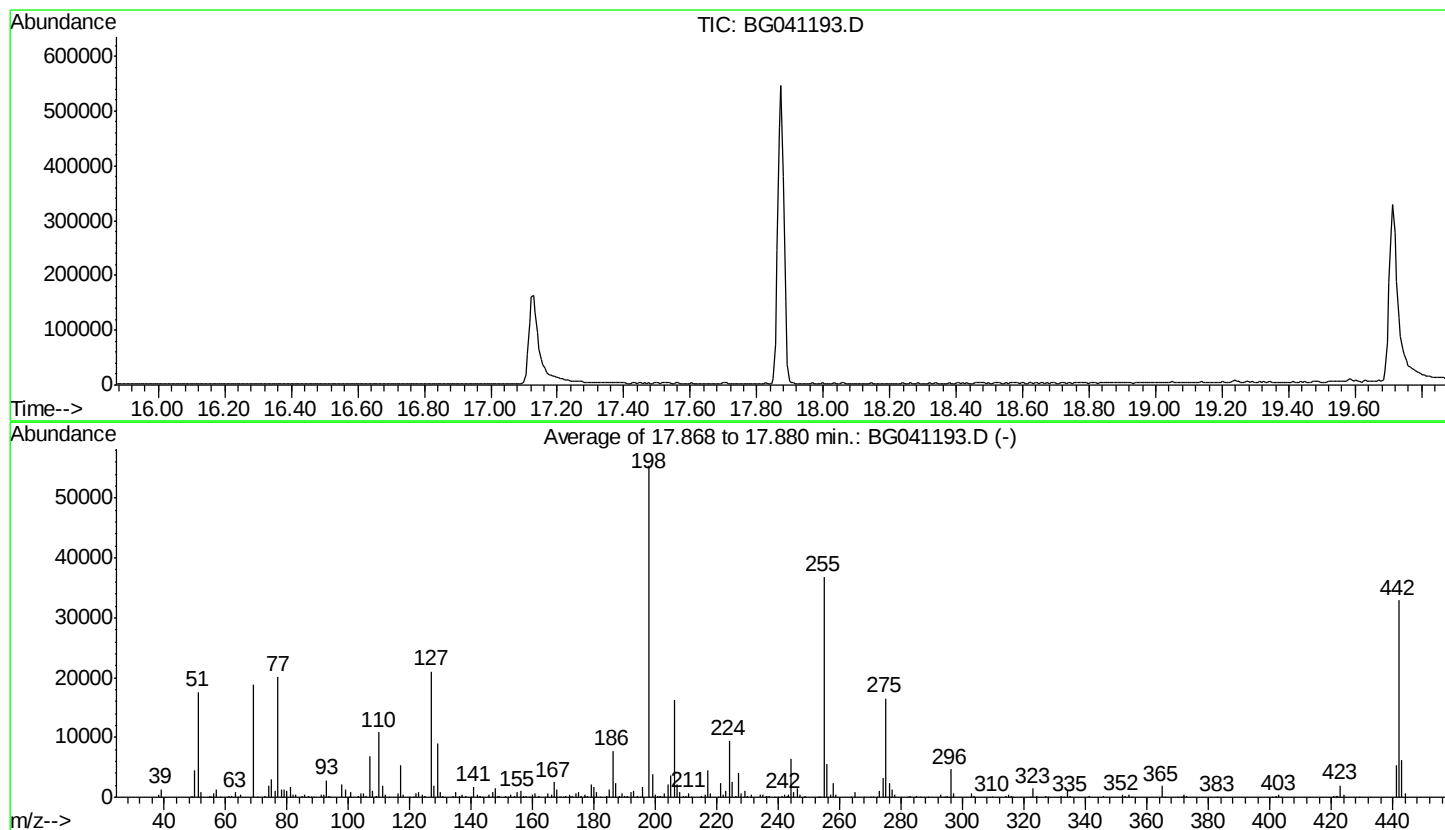

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	17594	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	18748	PASS
70	69	0.00	2	0.5	90	PASS
127	198	10	80	37.9	21018	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55442	PASS
199	198	5	9	6.8	3791	PASS
275	198	10	60	29.8	16515	PASS
365	198	1	100	3.4	1868	PASS
441	198	0.01	100	9.6	5335	PASS
442	198	50	100	59.4	32917	PASS
443	442	15	24	18.9	6208	PASS