


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061219\
 Data File : BG041209.D
 Acq On : 12 Jun 2019 16:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

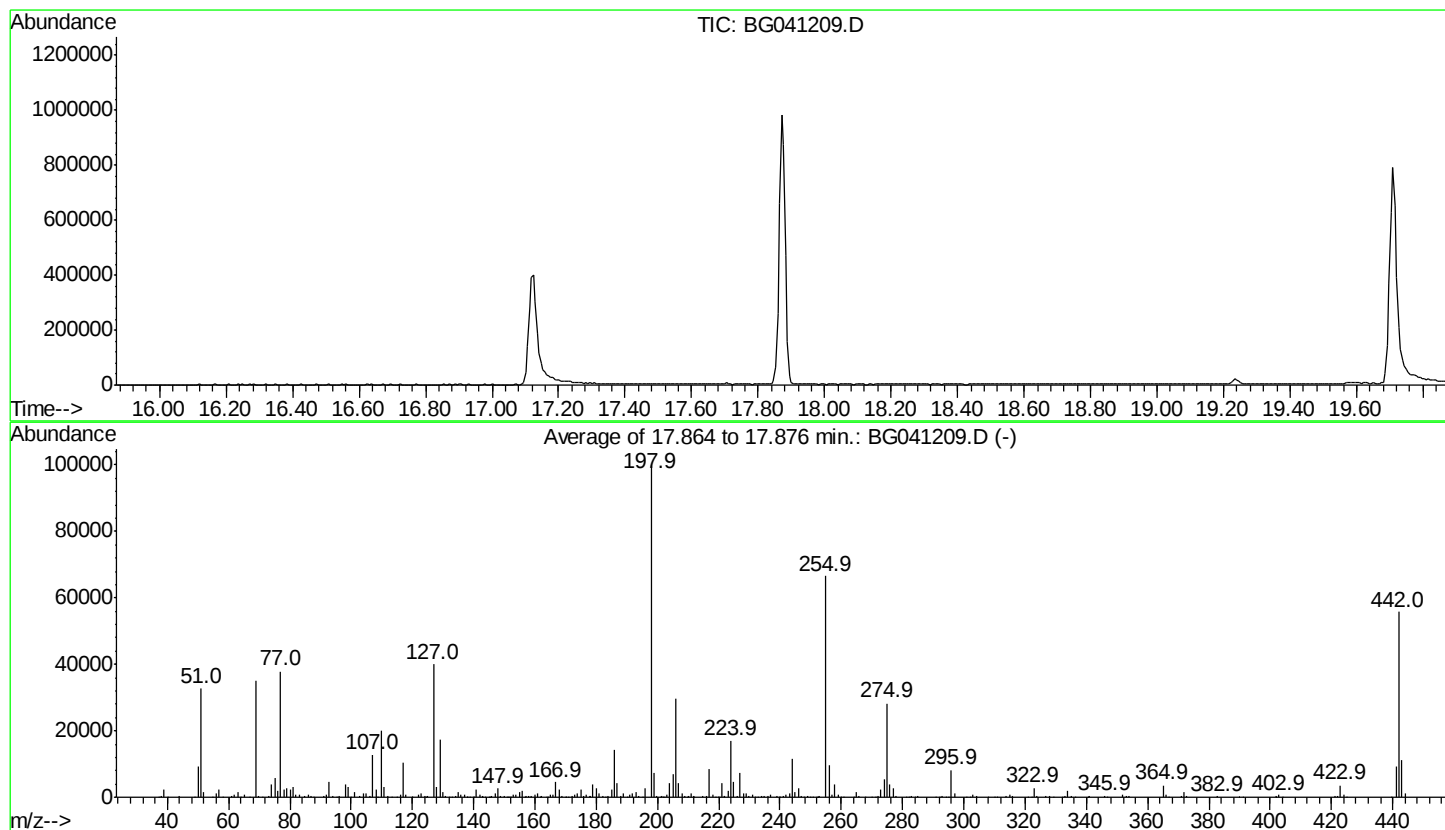

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	32640	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.0	34954	PASS
70	69	0.00	2	0.9	303	PASS
127	198	10	80	40.1	40040	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99805	PASS
199	198	5	9	7.2	7207	PASS
275	198	10	60	28.2	28178	PASS
365	198	1	100	3.7	3652	PASS
441	198	0.01	100	9.4	9357	PASS
442	198	50	100	55.9	55840	PASS
443	442	15	24	20.3	11321	PASS