
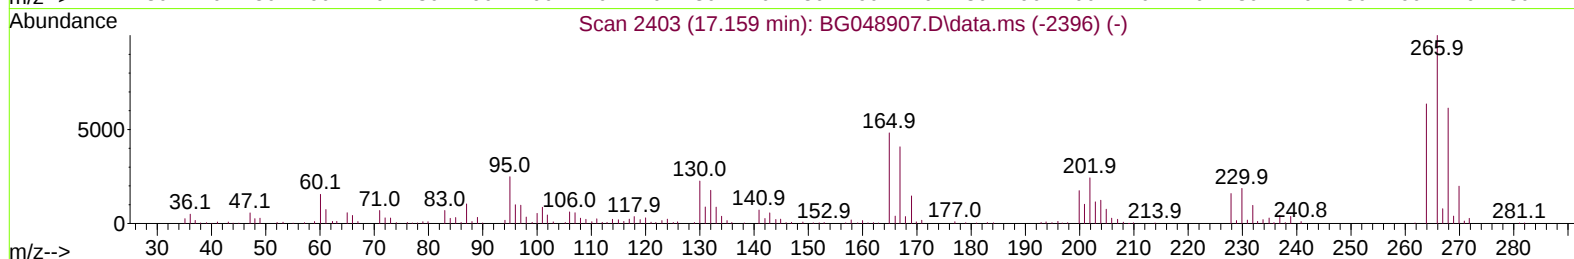
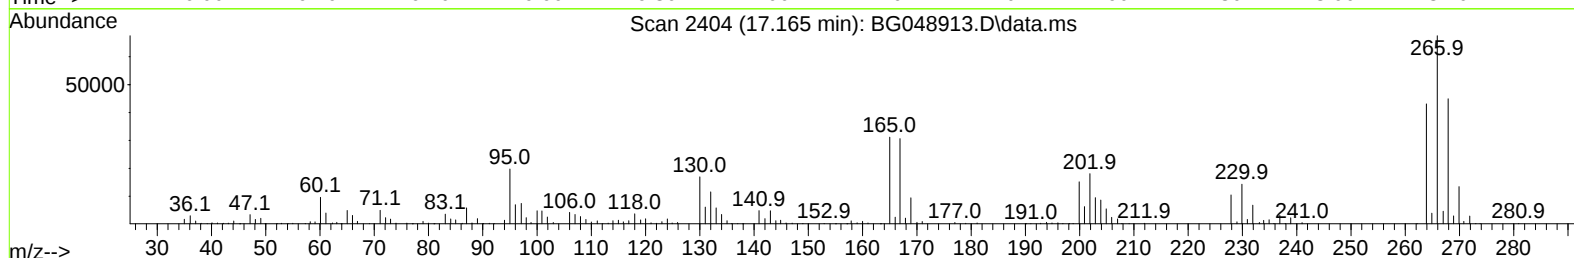


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
Data File : BG048913.D
Acq On : 12 Jun 2021 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 05:52:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

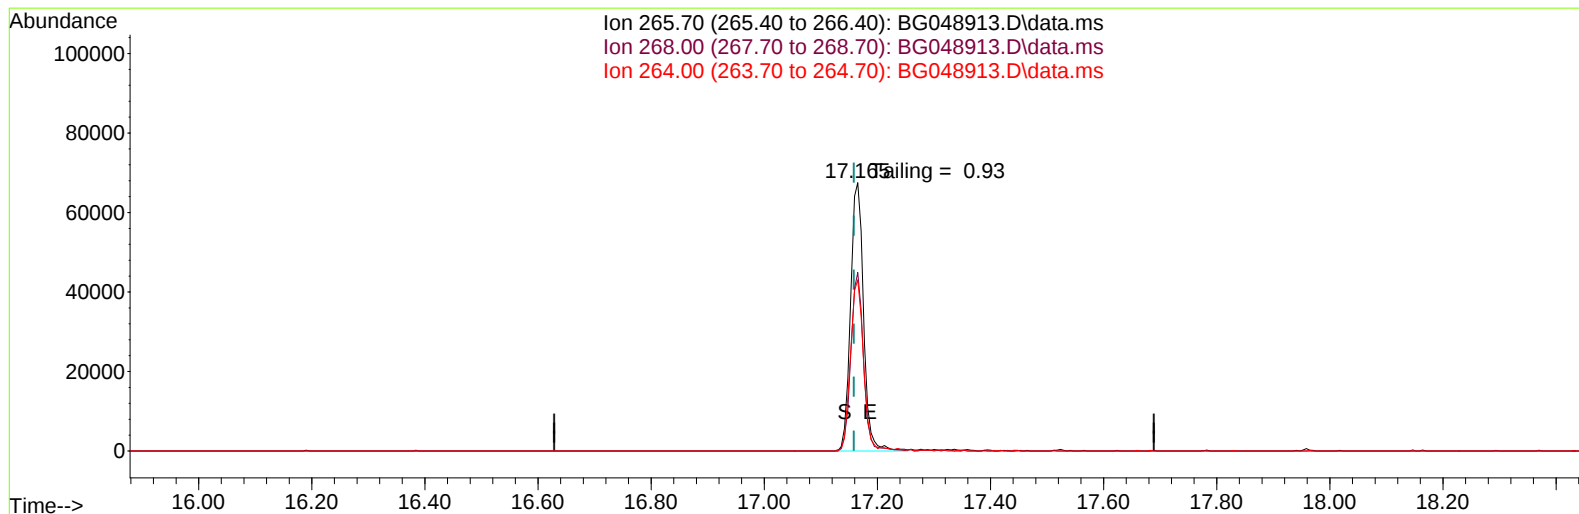

TIC: BG048913.D\data.ms

(70) Pentachlorophenol (C)




17.165min (+ 0.007) 235531.02 ng

response 107274

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	66.56
264.00	61.30	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048913.D
 Acq On : 12 Jun 2021 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 05:52:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

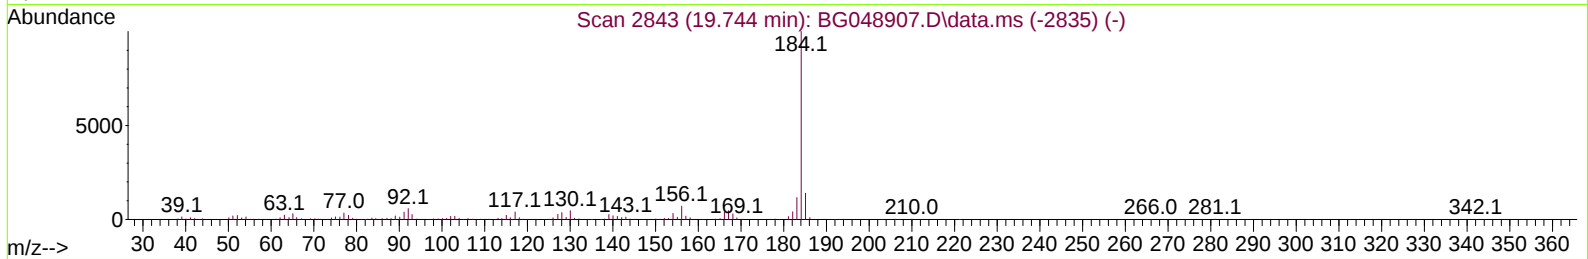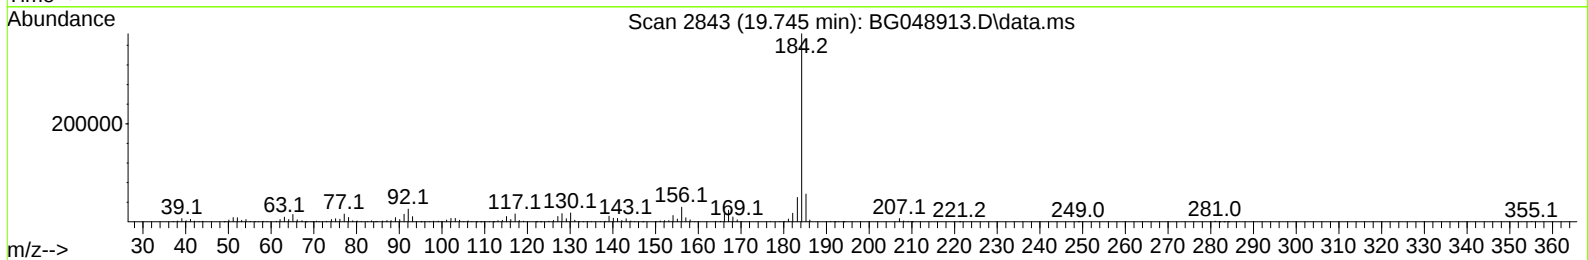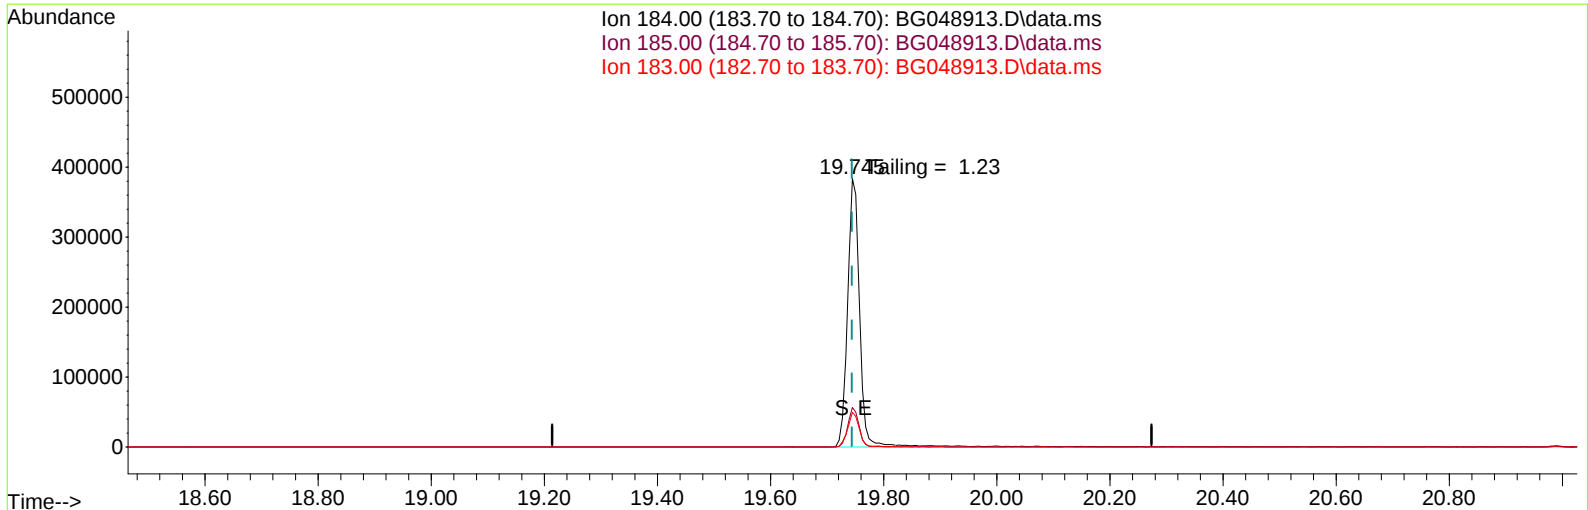

TIC: BG048913.D\data.ms

(77) Benzidine

19.745min (+ 0.001) 0.00 ng

response 559648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.74
183.00	11.70	12.98
0.00	0.00	0.00