

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048915.D
 Acq On : 12 Jun 2021 16:40
 Operator : CG/JU
 Sample : PB137054BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB137054BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.206	364	369	378	rBV	74186	124514	3.11%	0.783%
2	5.670	440	448	457	rBV	926234	1541640	38.50%	9.697%
3	7.268	710	720	731	rBV	924909	1635727	40.85%	10.289%
4	8.126	859	866	876	rVB	163526	286643	7.16%	1.803%
5	9.289	1056	1064	1075	rBV	569527	1025935	25.62%	6.453%
6	10.946	1336	1346	1354	rBV	209468	384662	9.61%	2.420%
7	13.390	1755	1762	1770	rVB	1407292	2217285	55.37%	13.947%
8	14.765	1988	1996	2005	rVB	342687	543317	13.57%	3.418%
9	16.252	2240	2249	2264	rBV	1185964	1814535	45.31%	11.414%
10	17.515	2458	2464	2473	rVB	468747	725420	18.12%	4.563%
11	19.824	2853	2857	2862	rVB3	36432	42036	1.05%	0.264%
12	20.123	2902	2908	2916	rBV	2816130	4004405	100.00%	25.188%
13	21.810	3188	3195	3202	rVB	473009	802693	20.05%	5.049%
14	25.147	3755	3763	3774	rVB2	254066	749109	18.71%	4.712%

Sum of corrected areas: 15897921

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
Data File : BG048915.D
Acq On : 12 Jun 2021 16:40
Operator : CG/JU
Sample : PB137054BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB137054BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.206	8.69 ng	124514	1,4-Dichlorobenzene-d4	8.126

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
4	1-Butene, 4-ethoxy-	100	C6H12O	044611-46-3	17		
5	Acetamide, N-(aminocarbonyl)-	102	C3H6N2O2	000591-07-1	9		

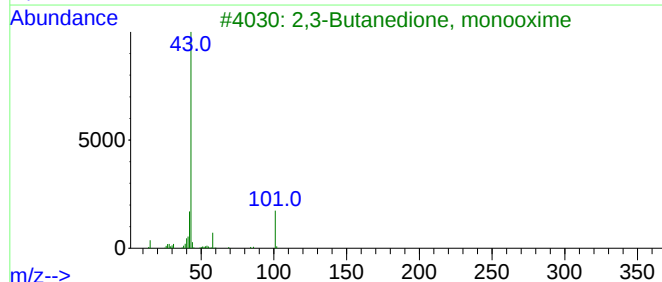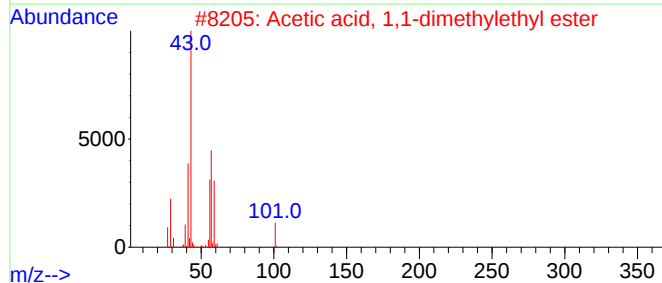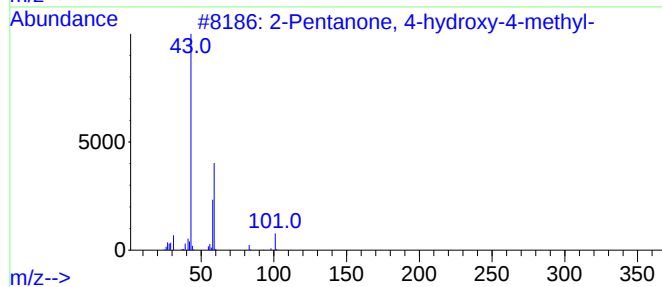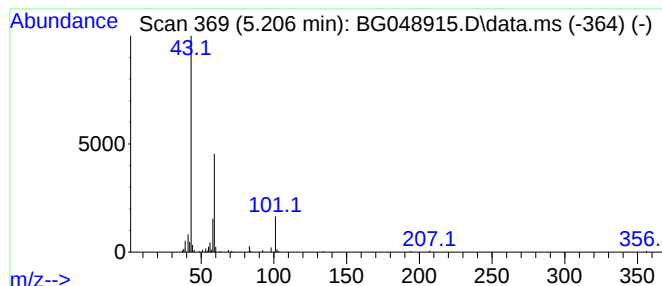

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
Data File : BG048915.D
Acq On : 12 Jun 2021 16:40
Operator : CG/JU
Sample : PB137054BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB137054BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.206	8.7	ng	124514	1	8.126	286643	20.0