
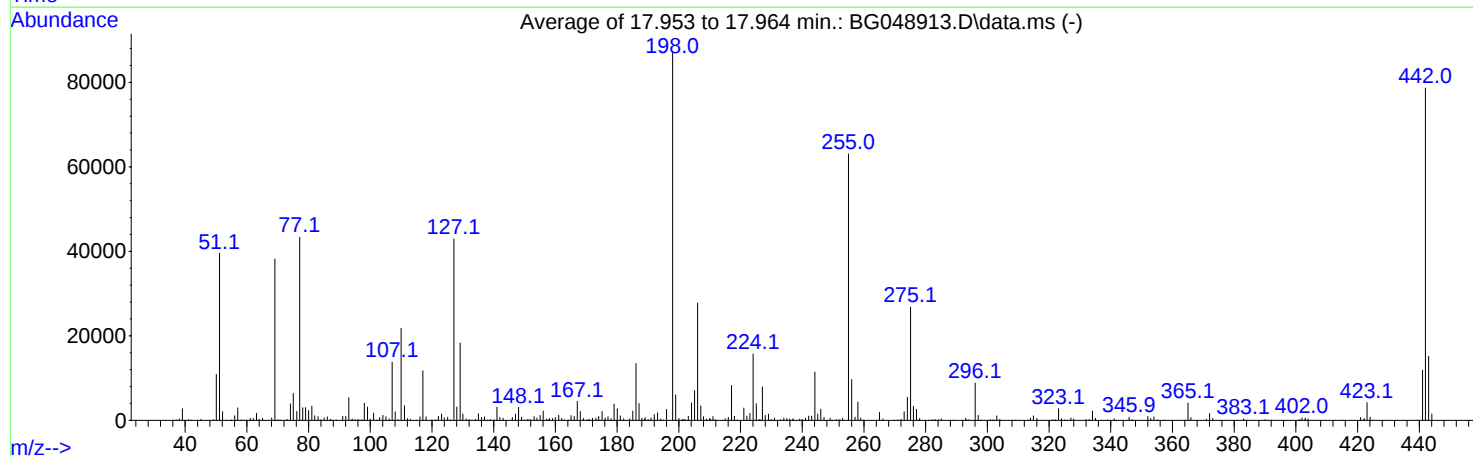


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048913.D
 Acq On : 12 Jun 2021 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 16:03:10 2021

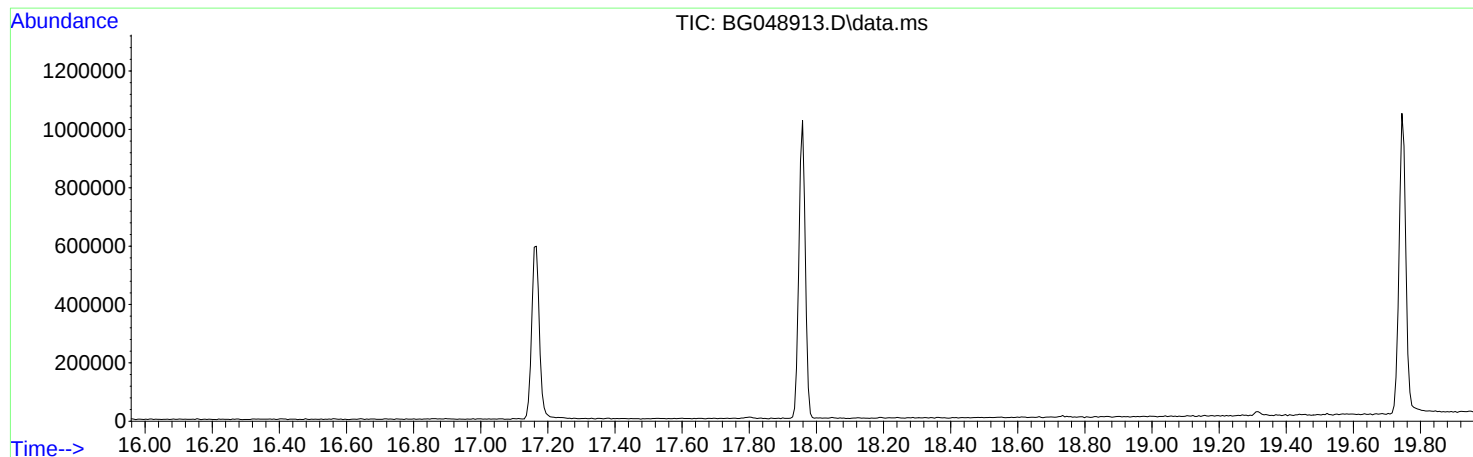




AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	39520	PASS
68	69	0.00	2	1.5	571	PASS
69	198	0.00	100	43.8	38171	PASS
70	69	0.00	2	0.5	202	PASS
127	198	10	80	49.3	42955	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87067	PASS
199	198	5	9	7.0	6077	PASS
275	198	10	60	30.8	26805	PASS
365	198	1	100	4.8	4150	PASS
441	198	0.01	100	13.6	11871	PASS
442	198	50	100	90.3	78645	PASS
443	442	15	24	19.3	15191	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048913.D
 Acq On : 12 Jun 2021 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 05:52:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

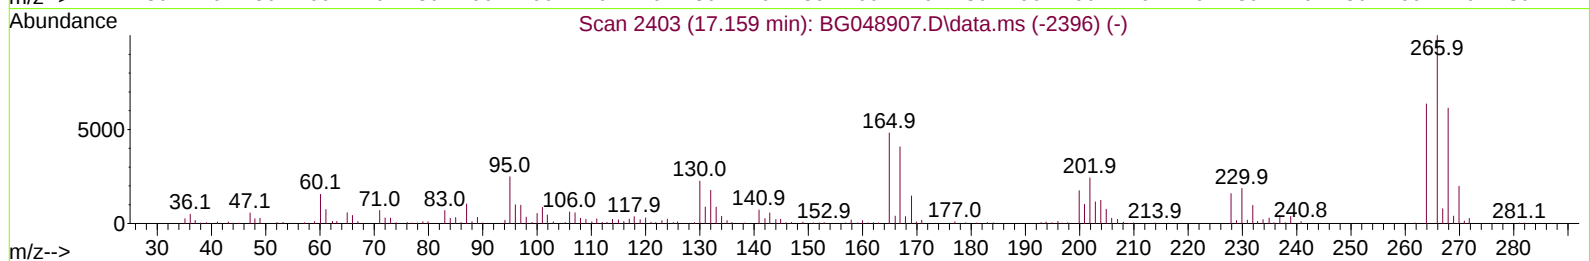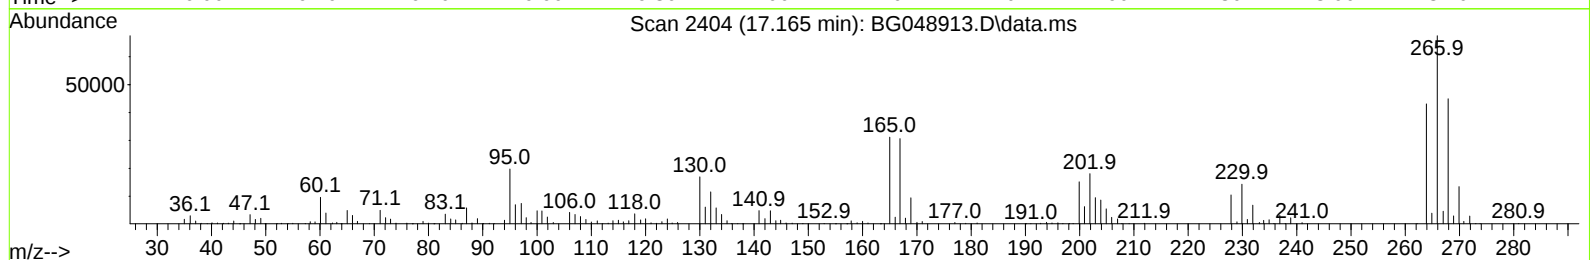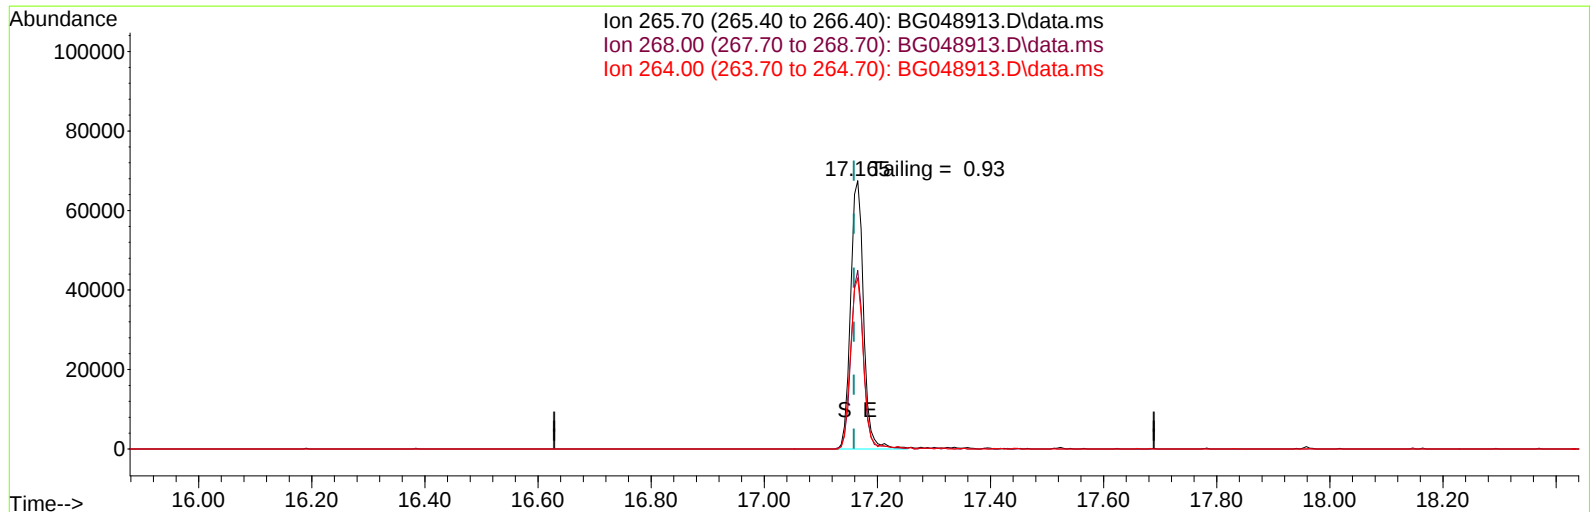

TIC: BG048913.D\data.ms

(70) Pentachlorophenol (C)

17.165min (+ 0.007) 235531.02 ng




response 107274

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	66.56
264.00	61.30	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048913.D
 Acq On : 12 Jun 2021 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 05:52:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

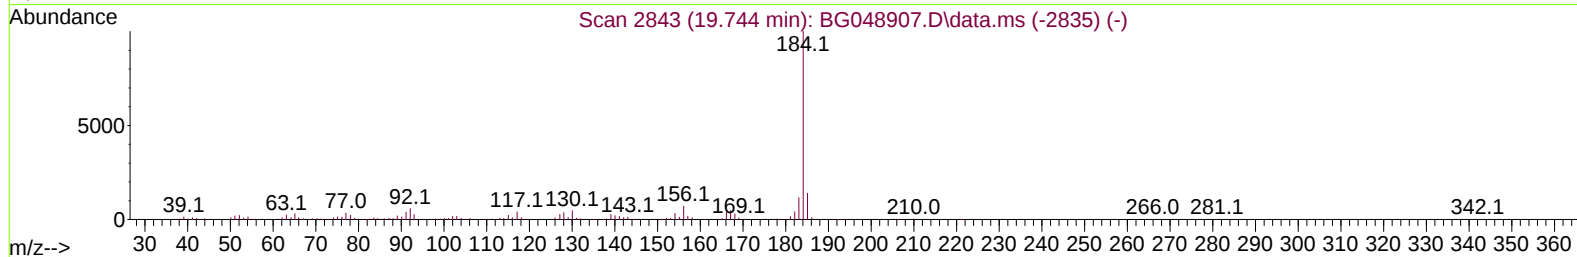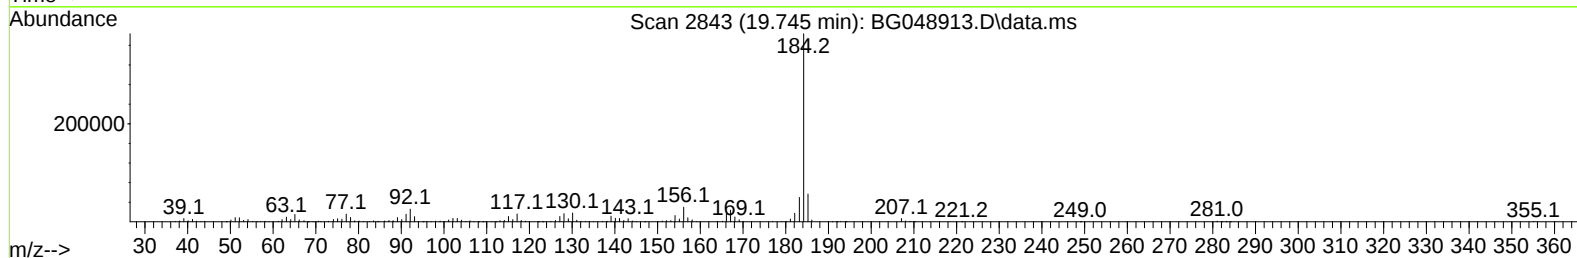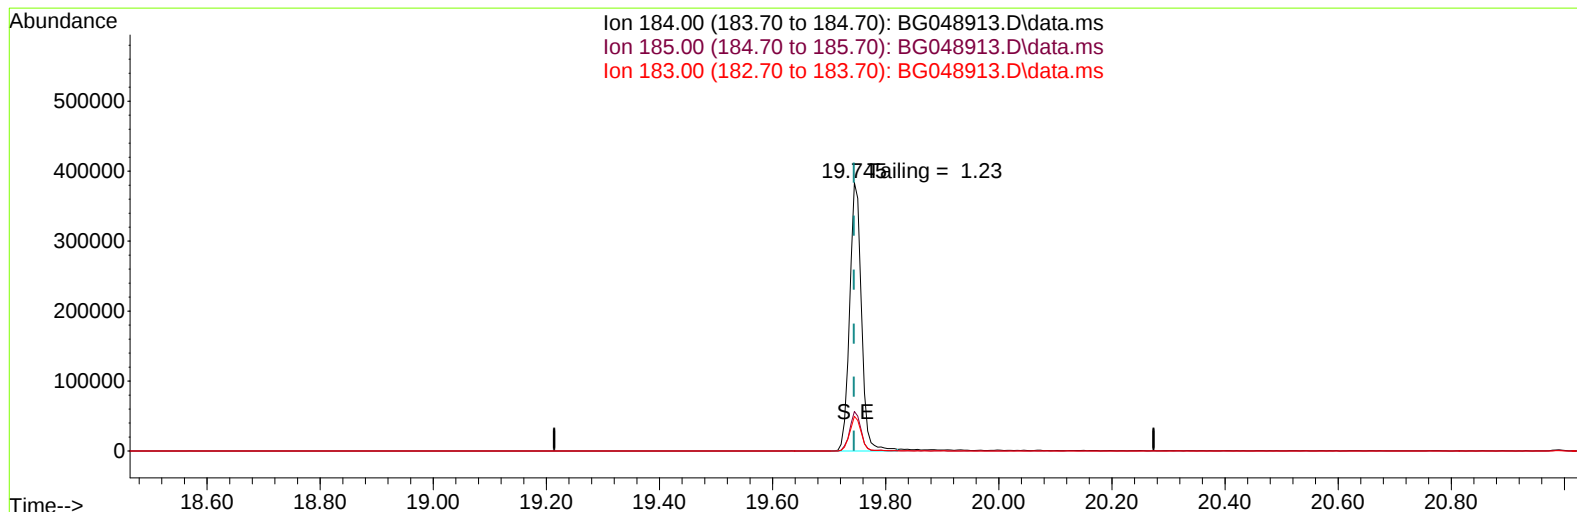

TIC: BG048913.D\data.ms

(77) Benzidine

19.745min (+ 0.001) 0.00 ng

response 559648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.74
183.00	11.70	12.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2021	BNA_G	BG048913.D
Compound Name	Response	Retention Time
DDT	288883	20.99
DDD	7209	20.538
DDE	546	20.038
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7755	296638	2.61

Instrument :
BNA_G
ClientSampleId :
DFTPP