


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048930.D
 Acq On : 13 Jun 2021 5:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 16:03:10 2021

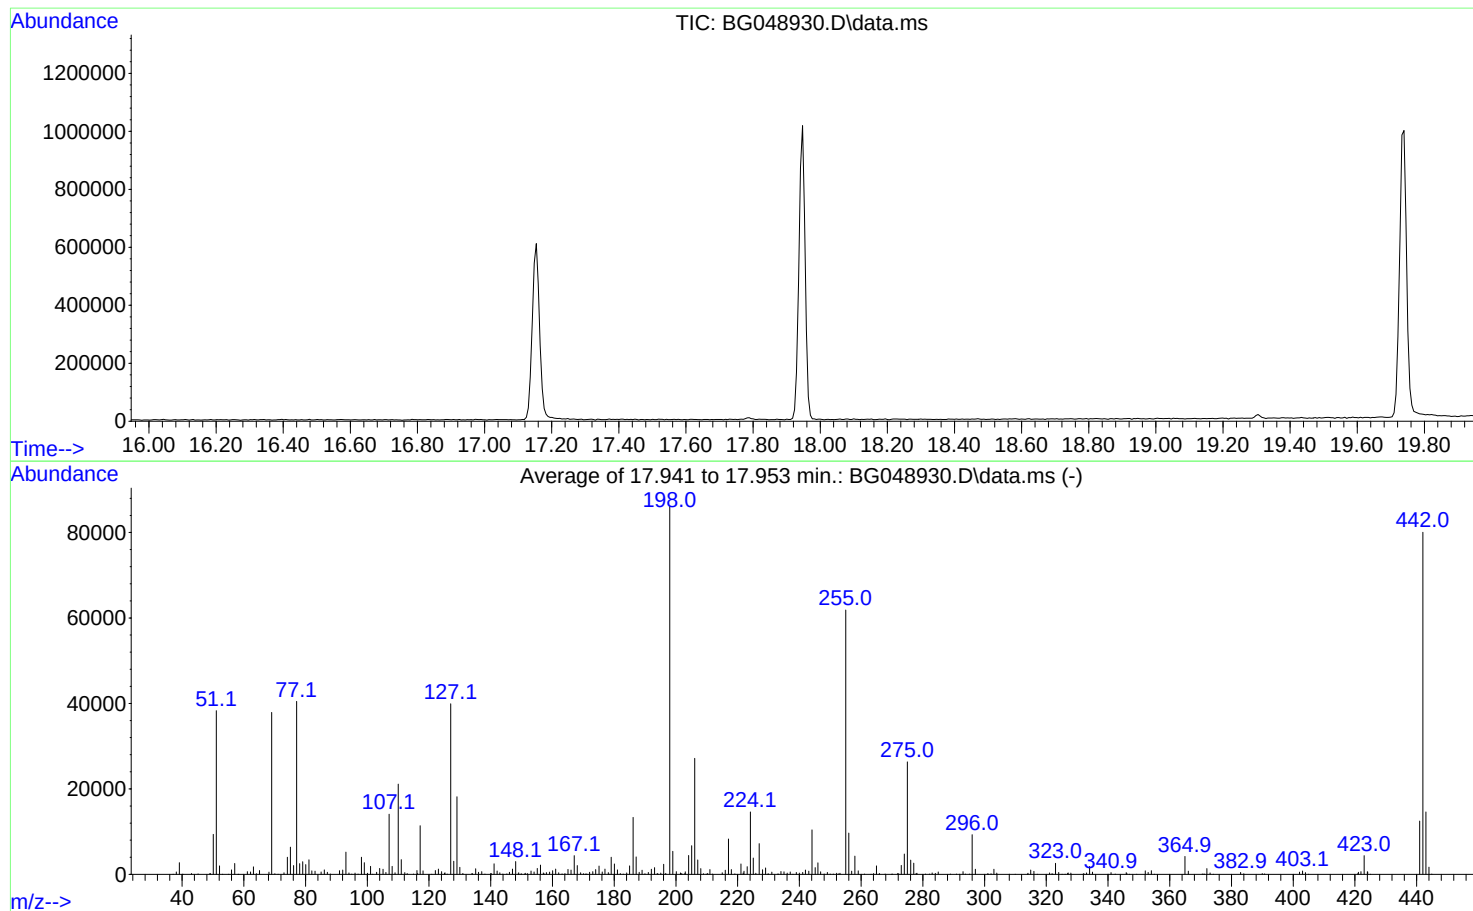




AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	38301	PASS
68	69	0.00	2	1.4	538	PASS
69	198	0.00	100	44.0	37877	PASS
70	69	0.00	2	0.4	160	PASS
127	198	10	80	46.4	39928	PASS
197	198	0.00	2	0.3	246	PASS
198	198	100	100	100.0	86083	PASS
199	198	5	9	6.3	5400	PASS
275	198	10	60	30.6	26315	PASS
365	198	1	100	4.9	4176	PASS
441	198	0.01	100	14.5	12454	PASS
442	198	50	100	93.0	80037	PASS
443	442	15	24	18.3	14613	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
 Data File : BG048930.D
 Acq On : 13 Jun 2021 5:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 05:56:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

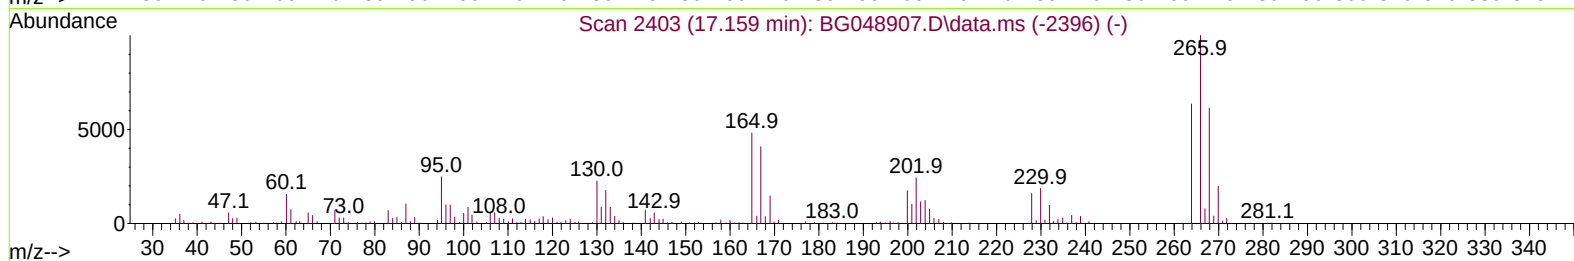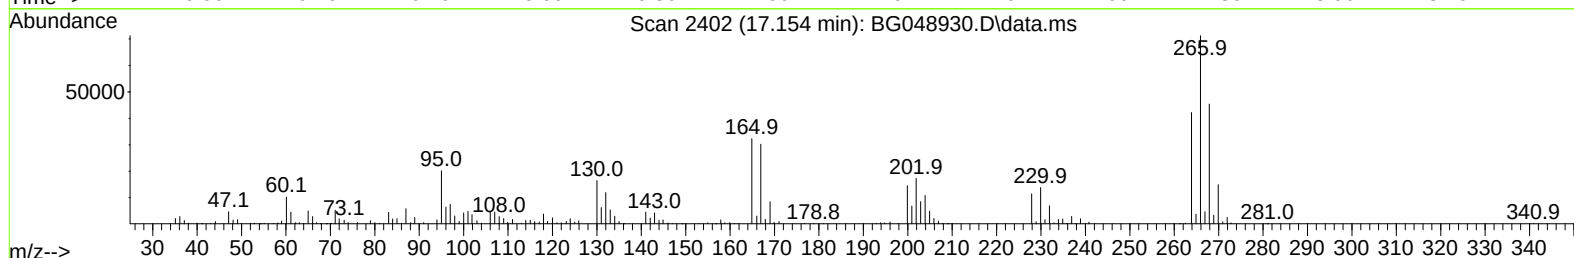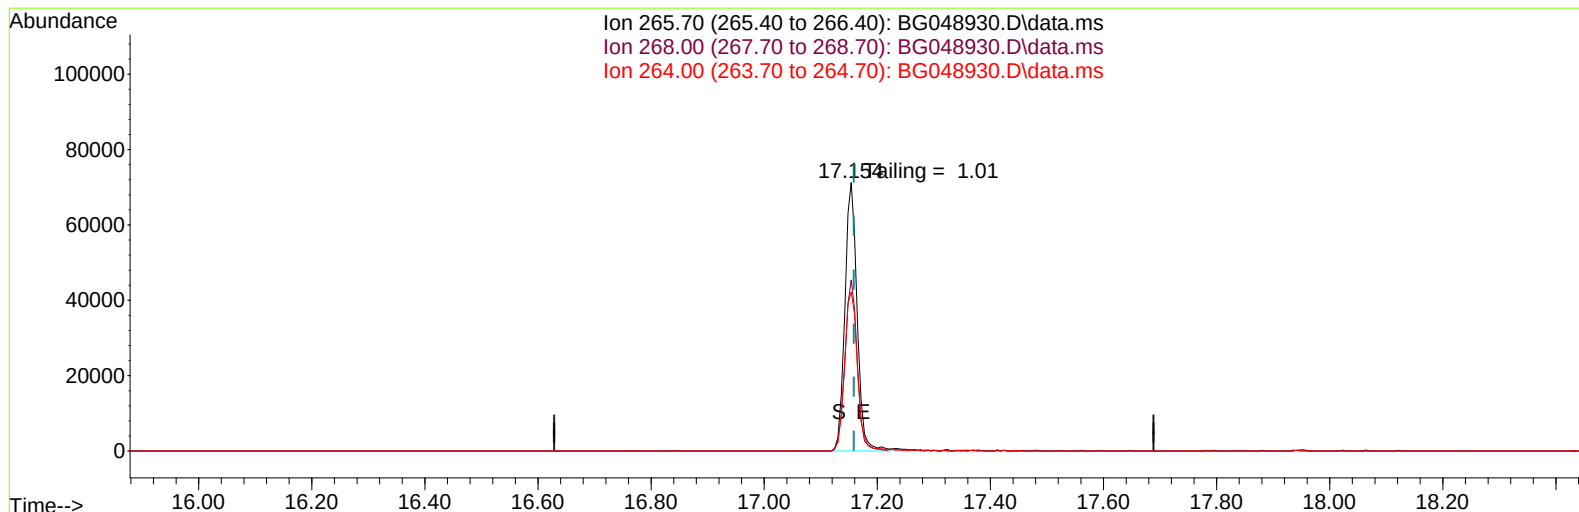

TIC: BG048930.D\data.ms

(70) Pentachlorophenol (C)

17.154min (-0.005) 0.00 ng




response 107228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.77
264.00	61.30	59.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061221\
Data File : BG048930.D
Acq On : 13 Jun 2021 5:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 14 05:56:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

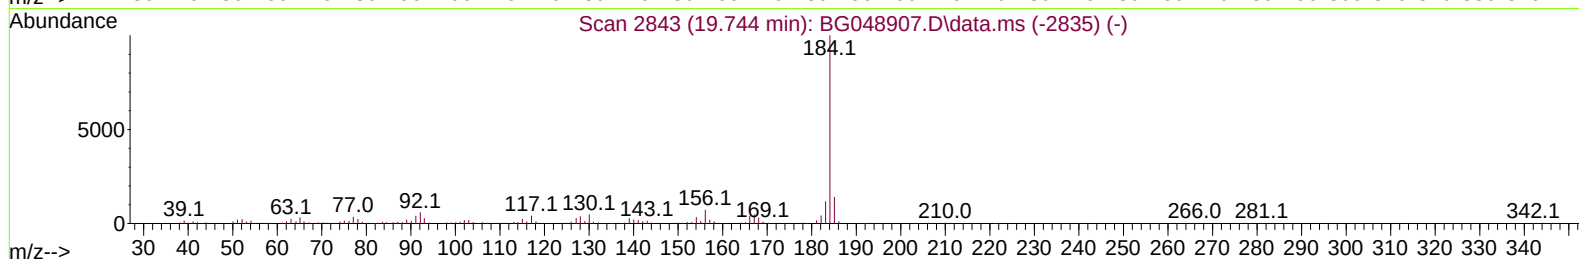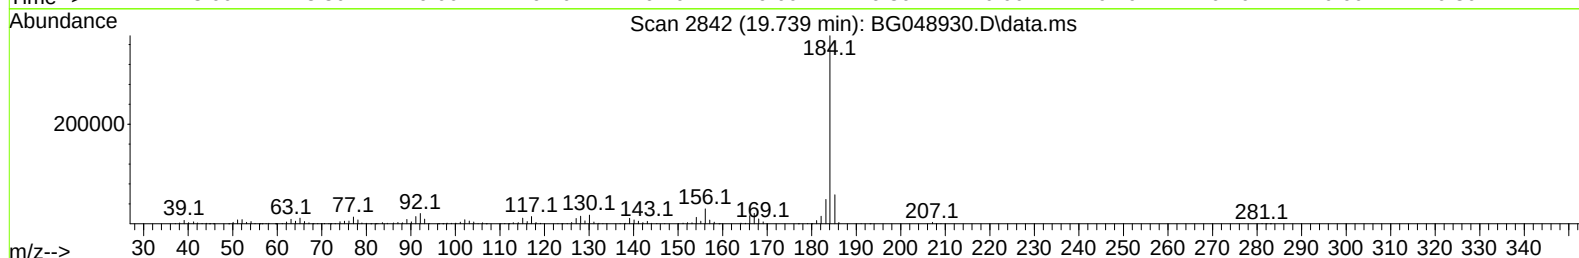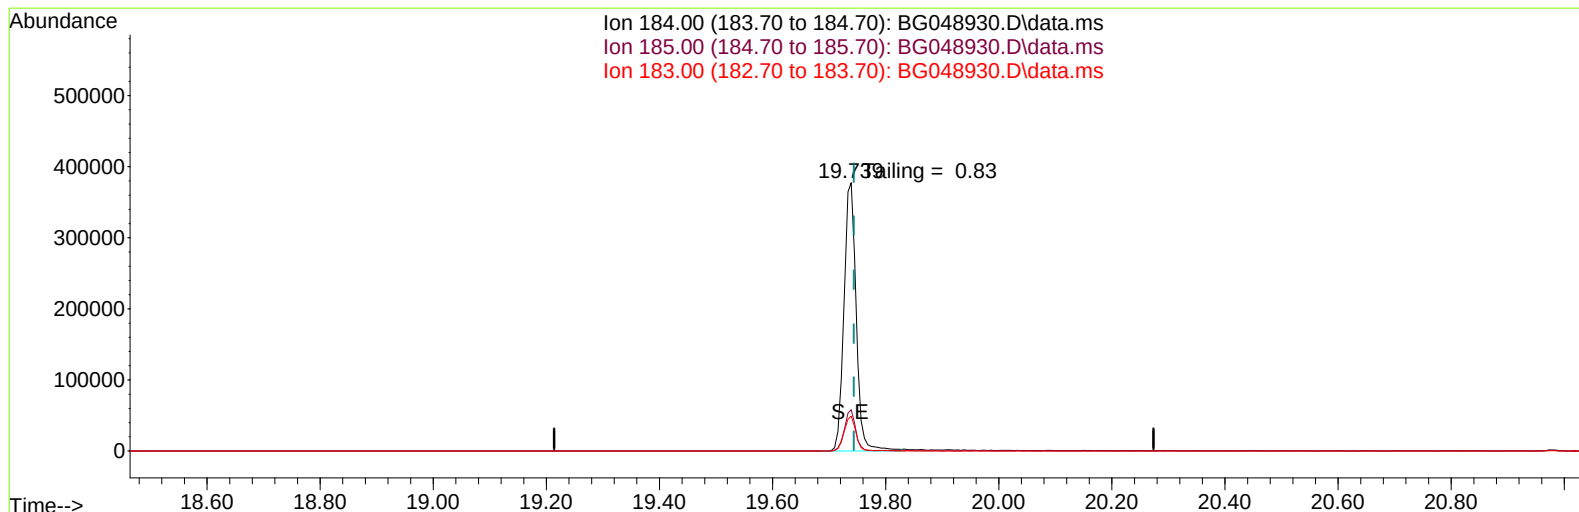

TIC: BG048930.D\data.ms

(77) Benzidine

19.739min (-0.005) 0.00 ng

response 570609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.41
183.00	11.70	12.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2021	BNA_G	BG048930.D
Compound Name	Response	Retention Time
DDT	298618	20.979
DDD	13369	20.526
DDE	882	20.027
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14251	312869	4.55

Instrument :
BNA_G
ClientSampleId :
DFTPP