
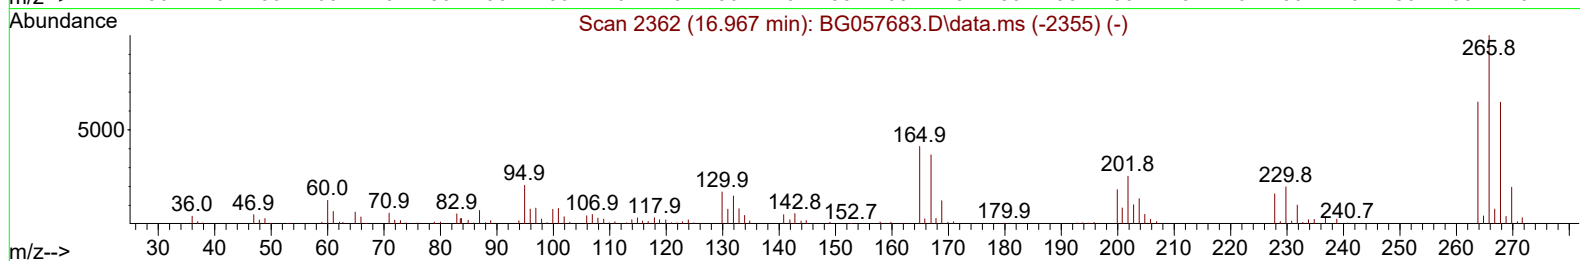
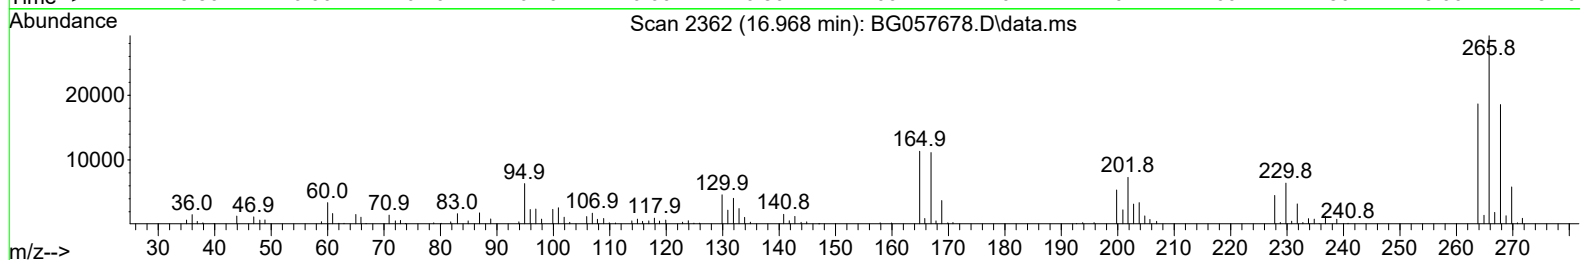


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
Data File : BG057678.D
Acq On : 12 Jun 2023 12:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 02:40:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 02:00:06 2023
Response via : Initial Calibration

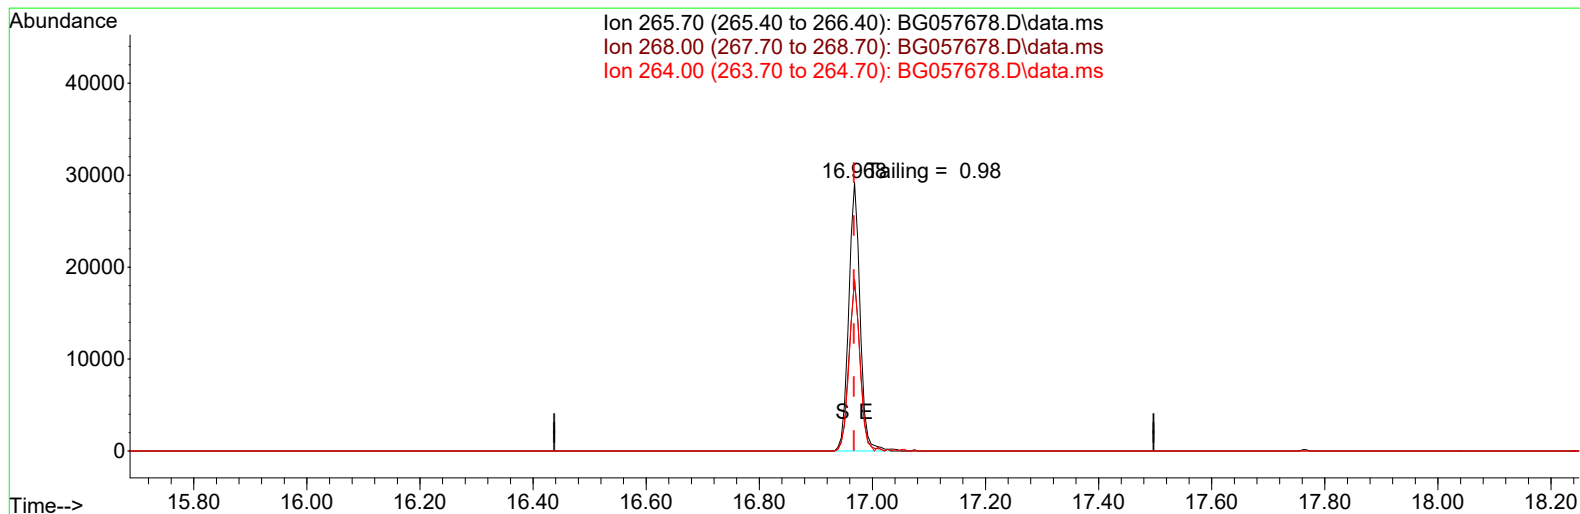

TIC: BG057678.D\data.ms

(70) Pentachlorophenol (C)




16.968min (+ 0.001) 18421.48 ng

response 40761

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.57
264.00	64.80	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
Data File : BG057678.D
Acq On : 12 Jun 2023 12:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 02:40:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 02:00:06 2023
Response via : Initial Calibration

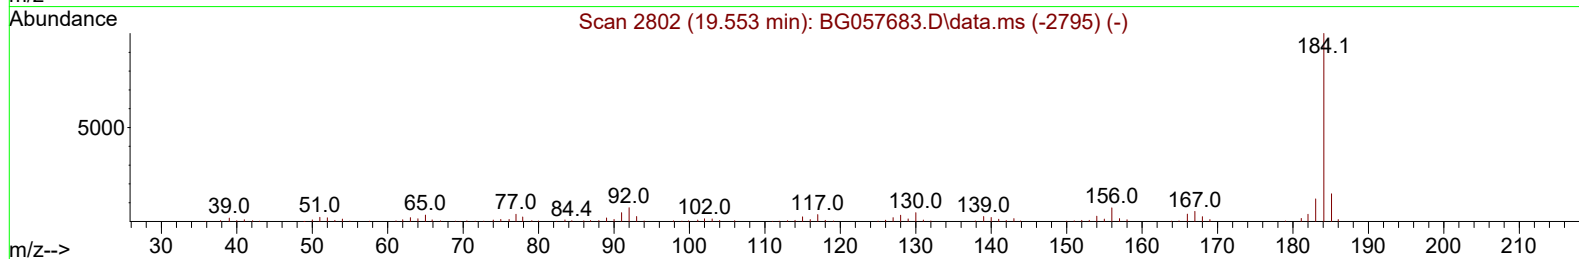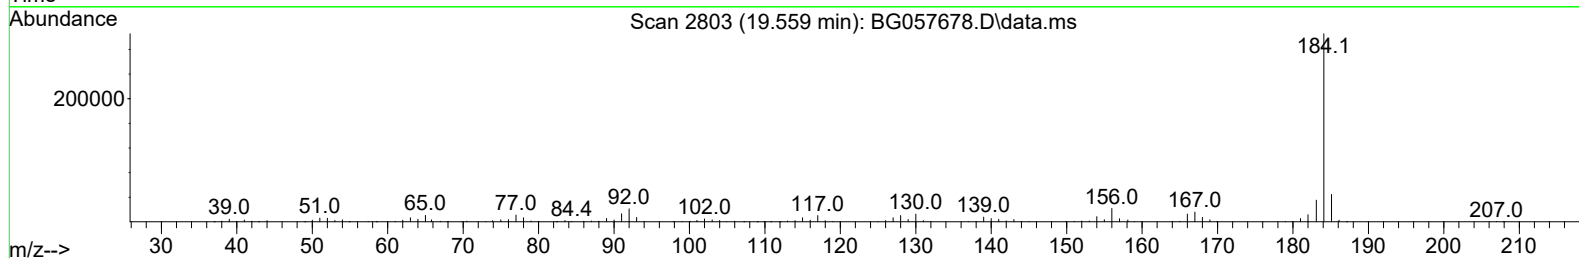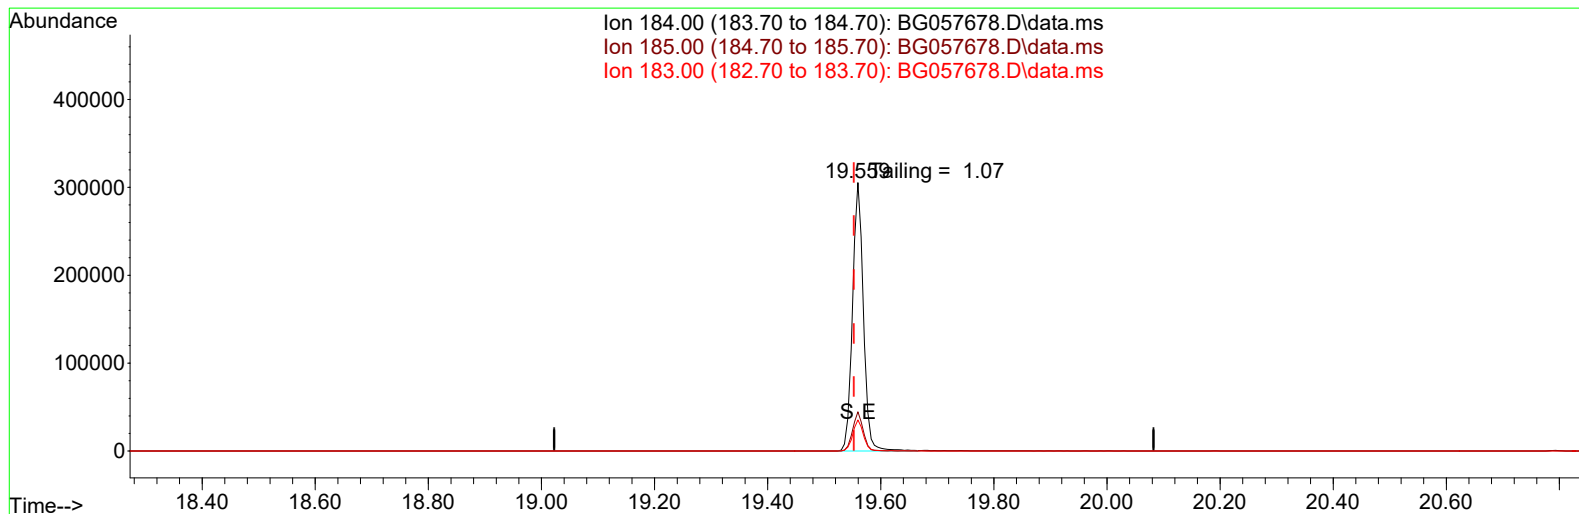

TIC: BG057678.D\data.ms

(77) Benzidine**19.559min (+ 0.007) 0.00 ng****response 408690**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.59
183.00	12.10	11.56
0.00	0.00	0.00