

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
 Data File : BG057688.D
 Acq On : 12 Jun 2023 19:28
 Operator : CG/JU
 Sample : PB153327BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB153327BL

Quant Time: Jun 13 02:21:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 13 02:00:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	28389	20.000	ng	0.00
21) Naphthalene-d8	10.744	136	118203	20.000	ng	0.00
39) Acenaphthene-d10	14.575	164	80795	20.000	ng	0.00
64) Phenanthrene-d10	17.318	188	203079	20.000	ng	0.00
76) Chrysene-d12	21.572	240	188929	20.000	ng	0.00
86) Perylene-d12	24.739	264	220674	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.515	112	332162	183.479	ng	0.00
7) Phenol-d6	7.101	99	450402	171.998	ng	0.00
23) Nitrobenzene-d5	9.104	82	254878	132.140	ng	0.00
42) 2,4,6-Tribromophenol	16.061	330	175839	178.433	ng	0.00
45) 2-Fluorobiphenyl	13.206	172	612075	109.751	ng	0.00
79) Terphenyl-d14	19.939	244	1144455	111.879	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
Data File : BG057688.D
Acq On : 12 Jun 2023 19:28
Operator : CG/JU
Sample : PB153327BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB153327BL

Quant Time: Jun 13 02:21:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 02:00:06 2023
Response via : Initial Calibration




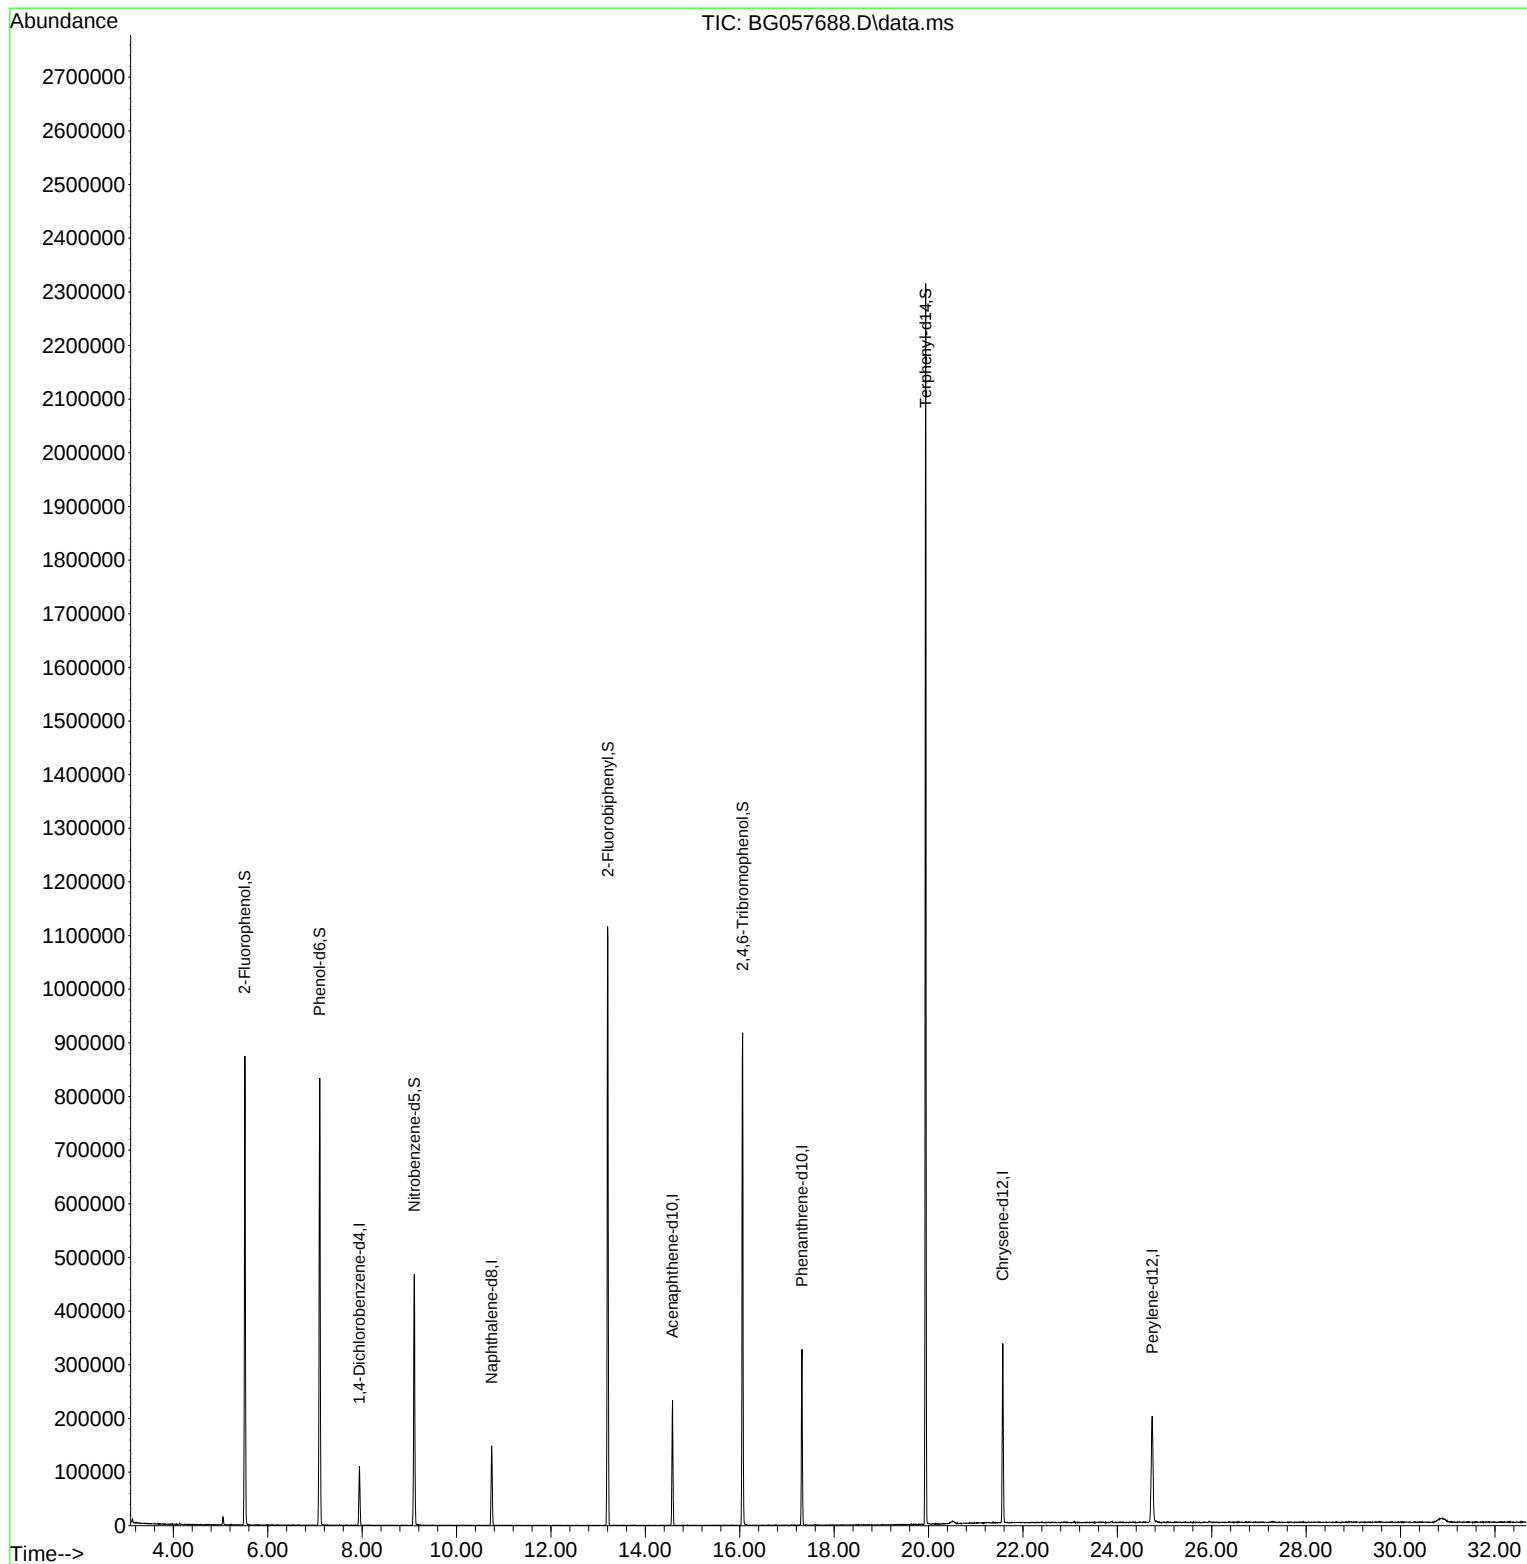




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.941 min Scan# 81
Delta R.T. -0.002 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28




Instrument :
BNA_G
ClientSampleId :
PB153327BL


Tgt Ion:152 Resp: 28389
Ion Ratio Lower Upper
152 100
150 148.2 123.8 185.6
115 62.2 49.3 73.9

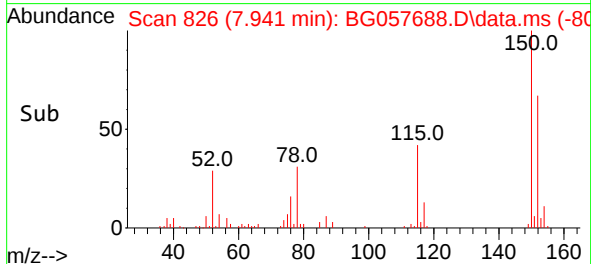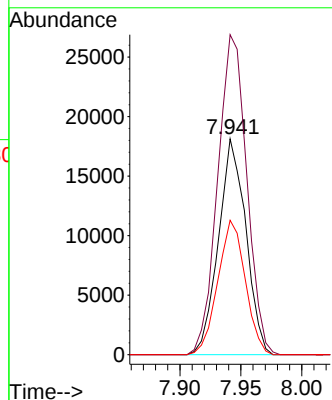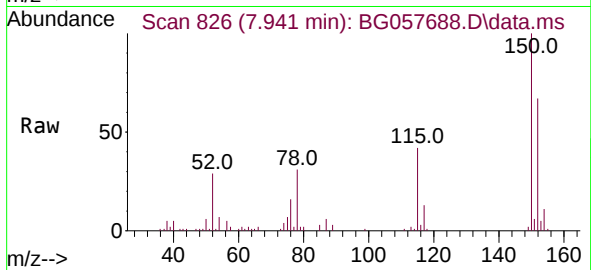

#5
2-Fluorophenol
Concen: 183.479 ng
RT: 5.515 min Scan# 413
Delta R.T. 0.004 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28

Tgt Ion:112 Resp: 332162
Ion Ratio Lower Upper
112 100
64 78.9 61.0 91.4
63 41.0 31.8 47.8


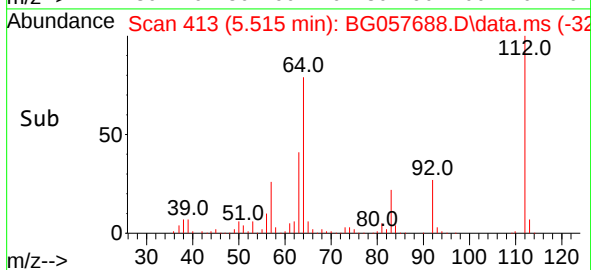
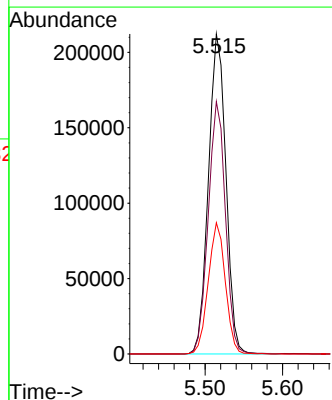
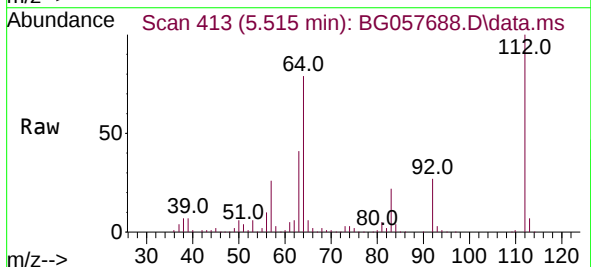


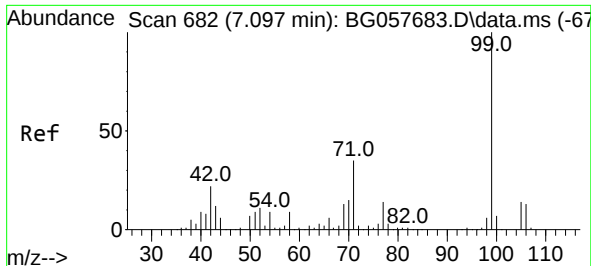

#7
Phenol-d6
Concen: 171.998 ng
RT: 7.101 min Scan# 61
Delta R.T. 0.004 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28




Instrument :
BNA_G
ClientSampleId :
PB153327BL


Tgt Ion: 99 Resp: 450402
Ion Ratio Lower Upper
99 100
42 23.0 17.9 26.9
71 35.4 28.3 42.5

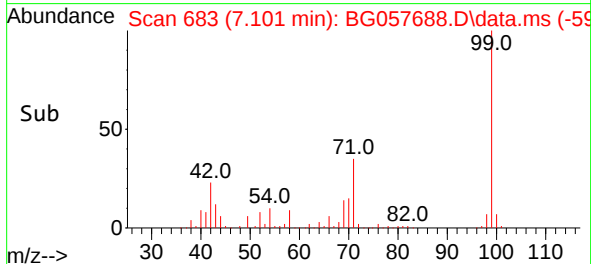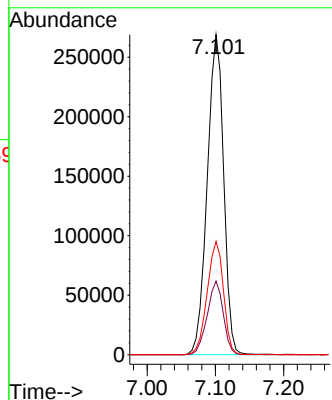

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.744 min Scan# 1303
Delta R.T. -0.007 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28

Tgt Ion: 136 Resp: 118203
Ion Ratio Lower Upper
136 100
137 11.1 8.6 13.0
54 13.6 10.3 15.5
68 6.9 6.3 9.5


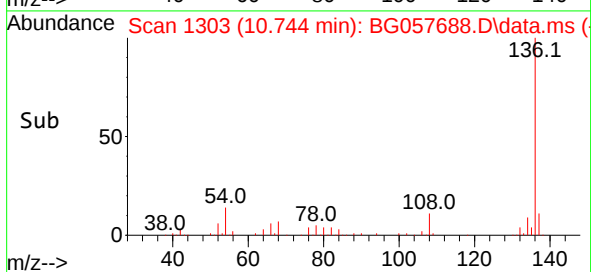
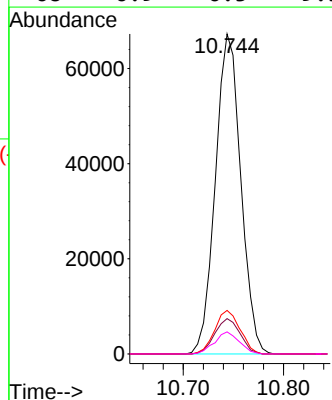
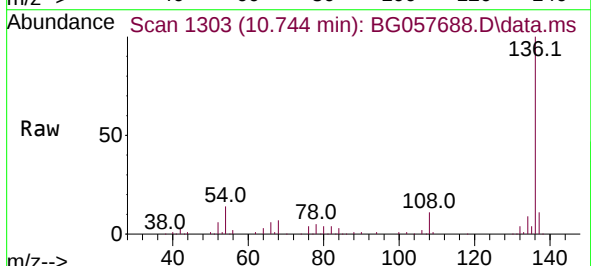


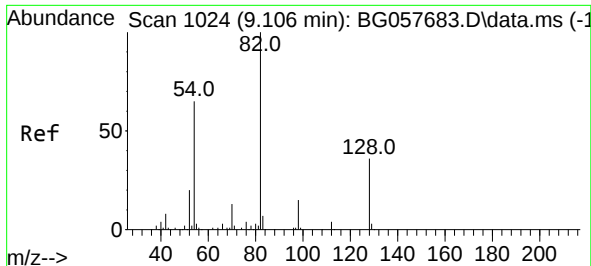

#23
Nitrobenzene-d5
Concen: 132.140 ng
RT: 9.104 min Scan# 1024
Delta R.T. -0.002 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28




Instrument :
BNA_G
ClientSampleId :
PB153327BL


Tgt Ion: 82 Resp: 254878
Ion Ratio Lower Upper
82 100
128 35.9 28.6 43.0
54 65.3 51.8 77.8

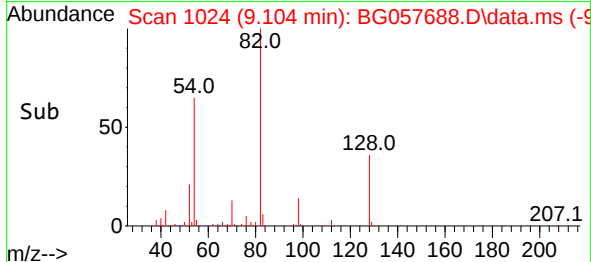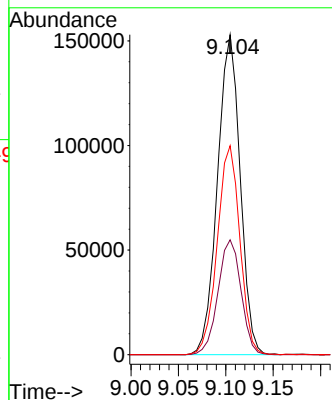

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.575 min Scan# 1955
Delta R.T. -0.007 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28


Tgt Ion:164 Resp: 80795
Ion Ratio Lower Upper
164 100
162 95.7 79.0 118.4
160 43.1 34.2 51.4

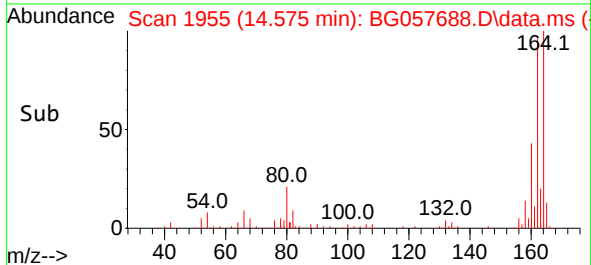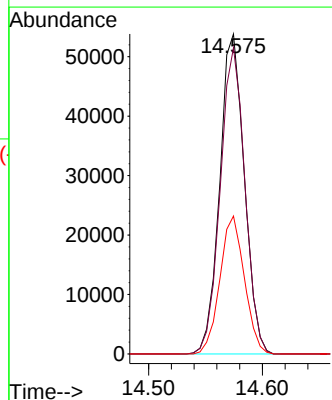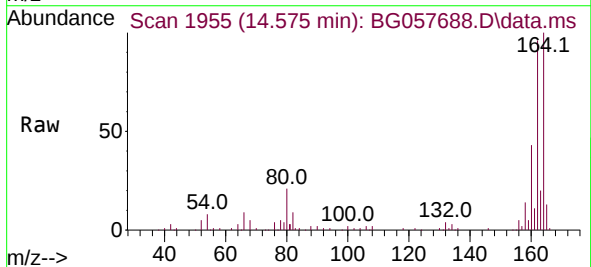



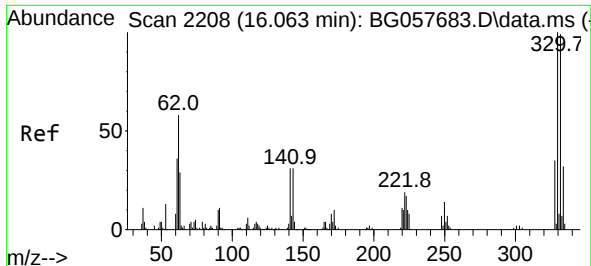


#42
2,4,6-Tribromophenol
Concen: 178.433 ng
RT: 16.061 min Scan# 21
Delta R.T. -0.002 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28

Instrument :
BNA_G
ClientSampleId :
PB153327BL







Tgt Ion:330 Resp: 175839
Ion Ratio Lower Upper
330 100
332 95.9 78.8 118.2
141 30.8 25.0 37.4

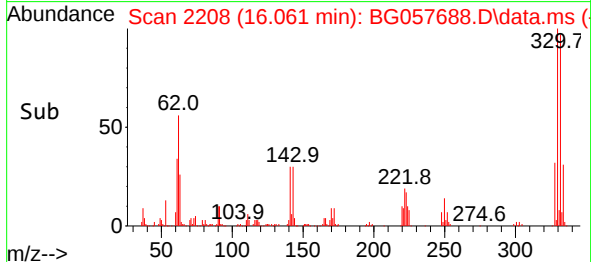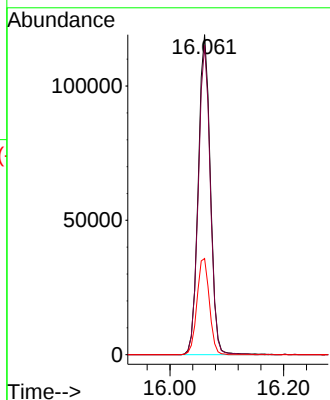

#45
2-Fluorobiphenyl
Concen: 109.751 ng
RT: 13.206 min Scan# 1722
Delta R.T. -0.002 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28

Tgt Ion:172 Resp: 612075
Ion Ratio Lower Upper
172 100
171 34.7 28.0 42.0
170 22.5 18.6 28.0


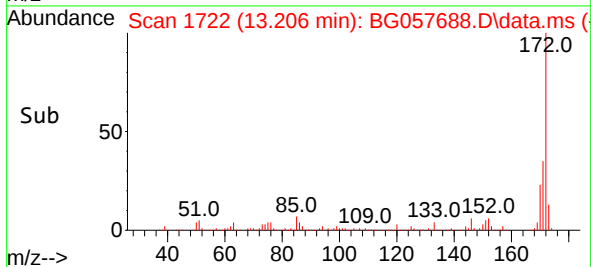
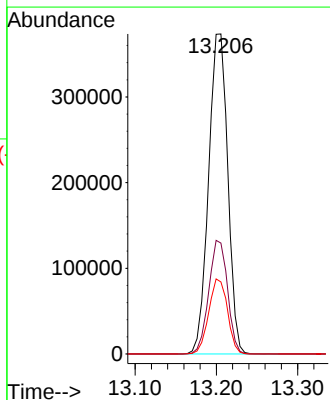
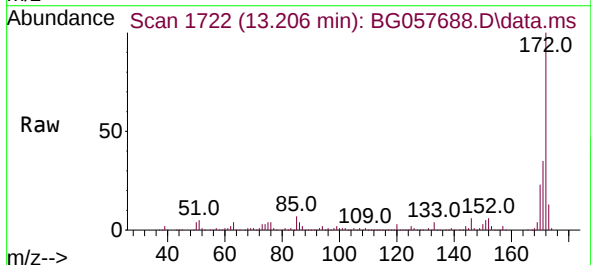


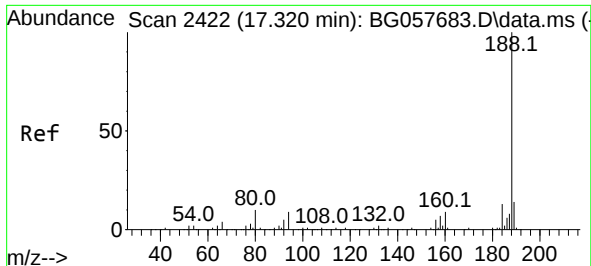

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.318 min Scan# 2422
Delta R.T. -0.002 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28




Instrument :
BNA_G
ClientSampleId :
PB153327BL


Tgt Ion:188 Resp: 203079
Ion Ratio Lower Upper
188 100
94 8.4 7.0 10.4
80 10.3 8.2 12.2

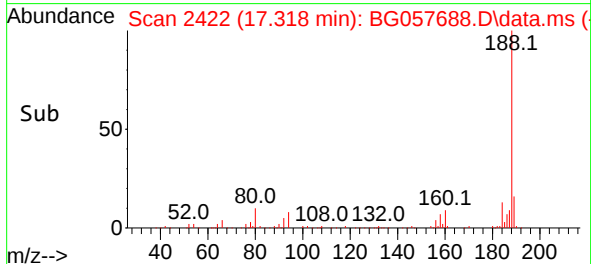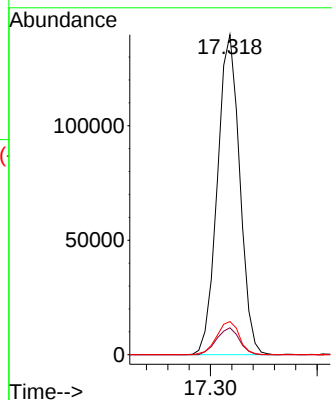

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.572 min Scan# 3146
Delta R.T. -0.007 min
Lab File: BG057688.D
Acq: 12 Jun 2023 19:28

Tgt Ion:240 Resp: 188929
Ion Ratio Lower Upper
240 100
120 8.7 7.6 11.4
236 26.6 20.9 31.3


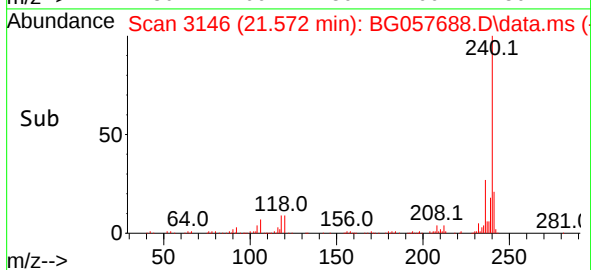
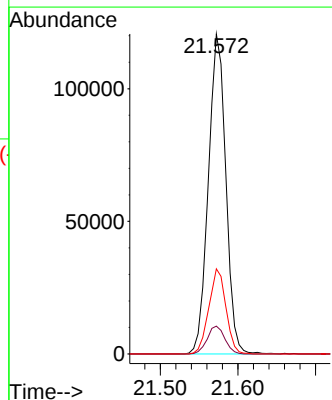
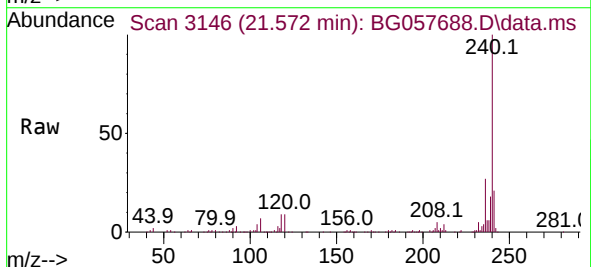


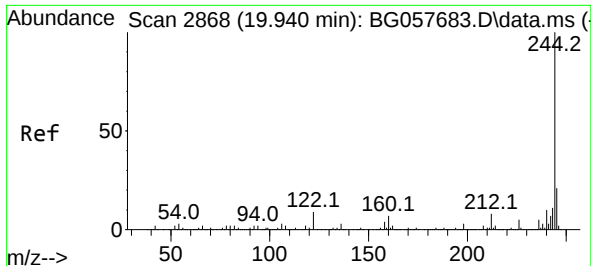

#79
 Terphenyl-d14
 Concen: 111.879 ng
 RT: 19.939 min Scan# 21
 Delta R.T. -0.002 min
 Lab File: BG057688.D
 Acq: 12 Jun 2023 19:28

Instrument :
 BNA_G
 ClientSampleId :
 PB153327BL

Tgt Ion:244 Resp: 1144455
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.2 9.4
 122 9.0 7.0 10.6

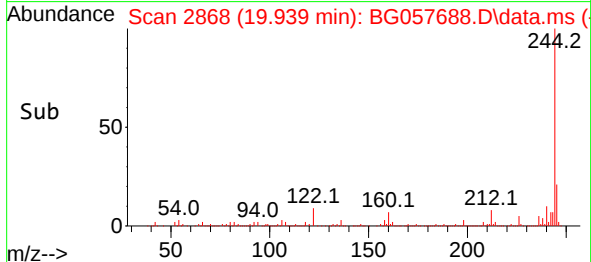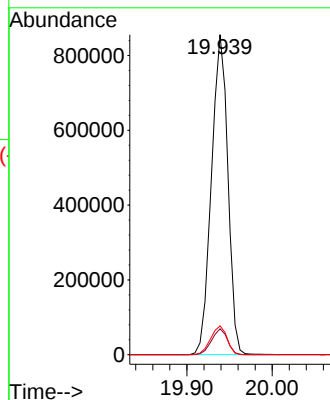

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.739 min Scan# 3685
 Delta R.T. -0.013 min
 Lab File: BG057688.D
 Acq: 12 Jun 2023 19:28

Tgt Ion:264 Resp: 220674
 Ion Ratio Lower Upper
 264 100
 260 23.0 17.6 26.4
 265 21.5 17.4 26.0

