
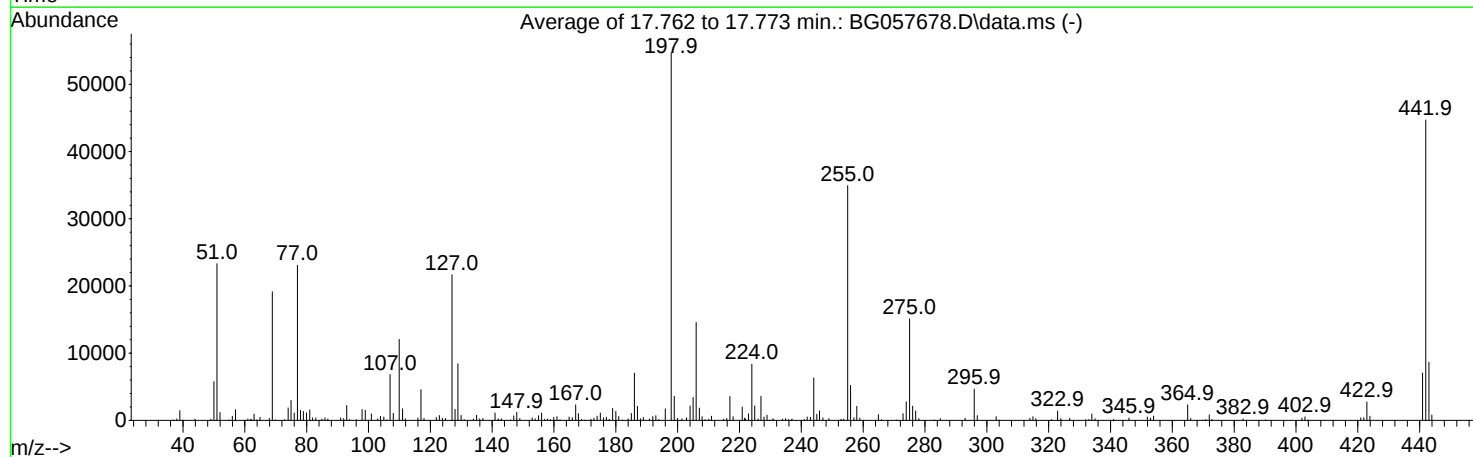


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
Data File : BG057678.D
Acq On : 12 Jun 2023 12:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 13 02:00:06 2023

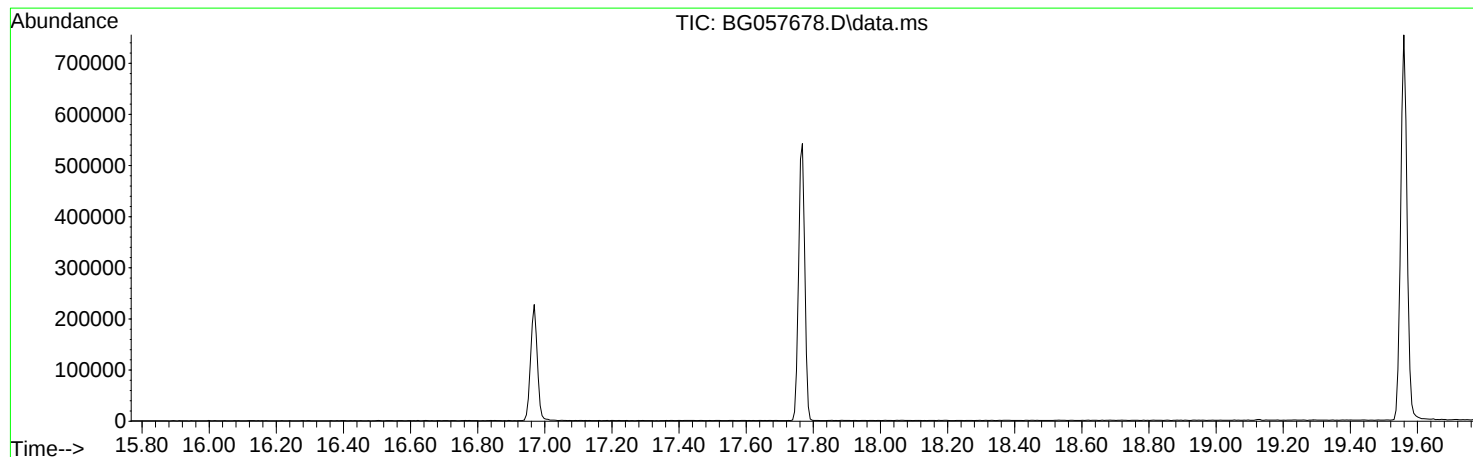

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	23301	PASS
68	69	0.00	2	1.6	304	PASS
69	198	0.00	100	35.0	19141	PASS
70	69	0.00	2	0.3	64	PASS
127	198	10	80	39.6	21670	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54739	PASS
199	198	5	9	6.5	3567	PASS
275	198	10	60	27.6	15126	PASS
365	198	1	100	4.2	2314	PASS
441	198	0.01	100	12.8	7027	PASS
442	442	50	100	100.0	44680	PASS
443	442	15	24	19.3	8639	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/12/2023	BNA_G	<u>BG057678.D</u>
Compound Name	Response	Retention Time
DDT	108988	20.793
DDD	1137	20.4
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1137	110125	1.03

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
Data File : BG057678.D
Acq On : 12 Jun 2023 12:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 13 02:40:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 02:00:06 2023
Response via : Initial Calibration

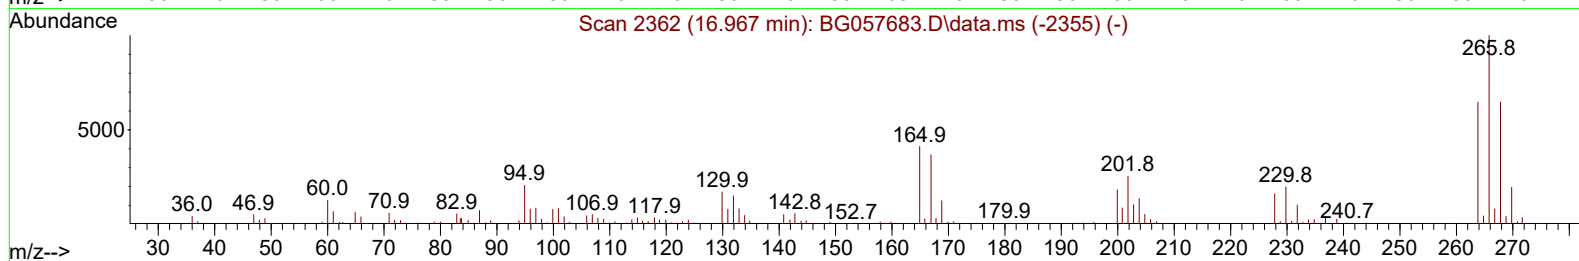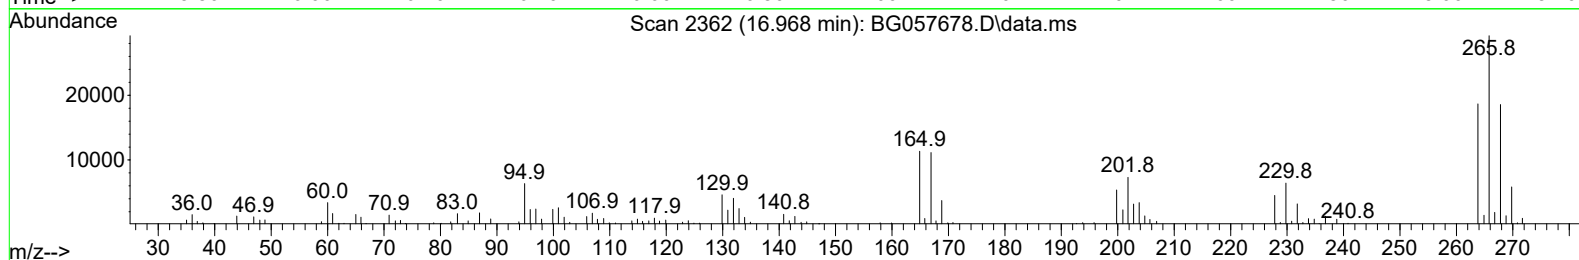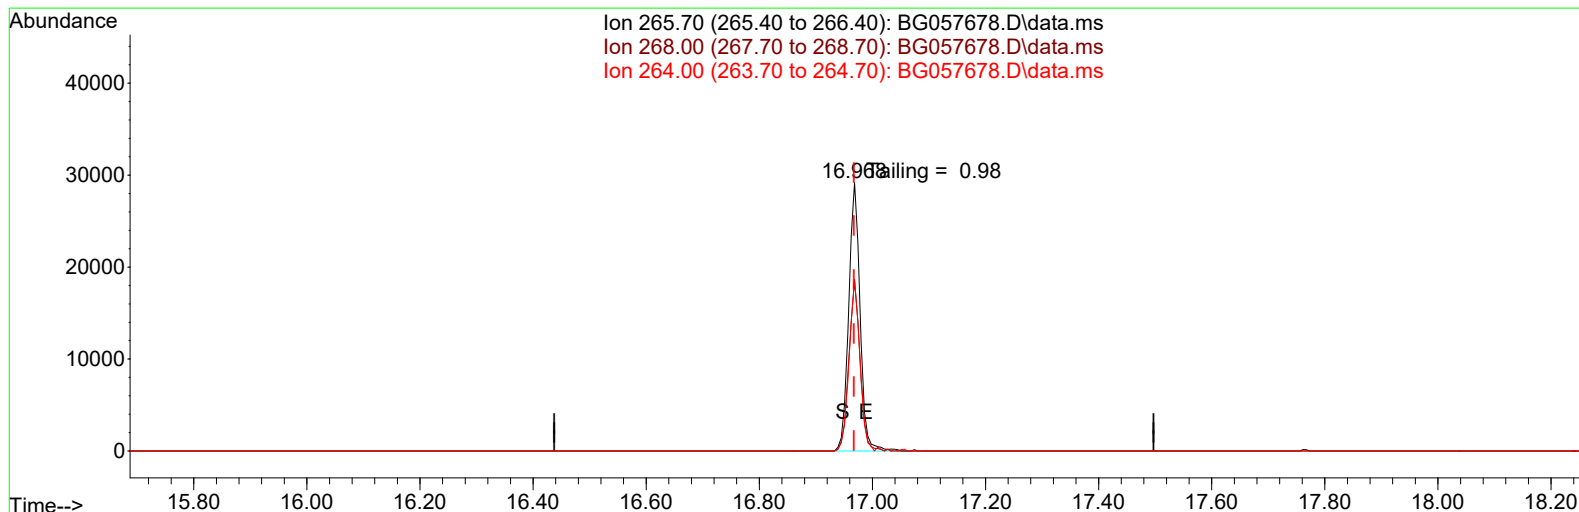

TIC: BG057678.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.001) 18421.48 ng




response 40761

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.57
264.00	64.80	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061223\
Data File : BG057678.D
Acq On : 12 Jun 2023 12:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 13 02:40:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 02:00:06 2023
Response via : Initial Calibration

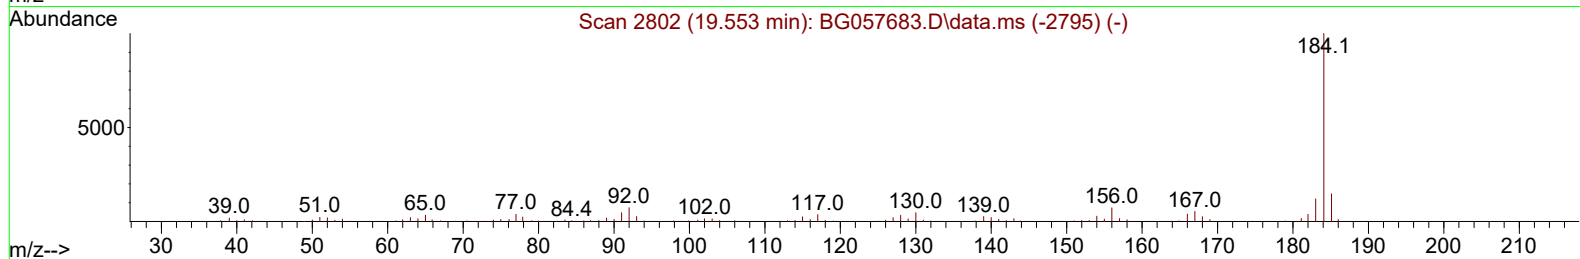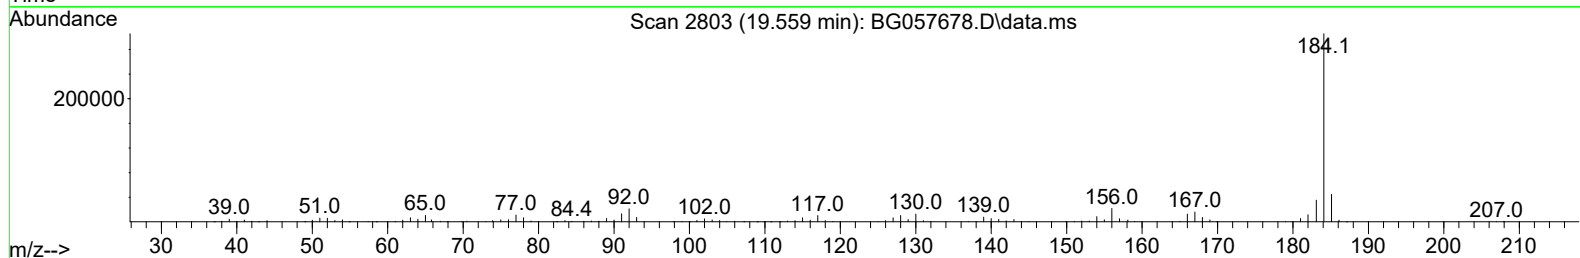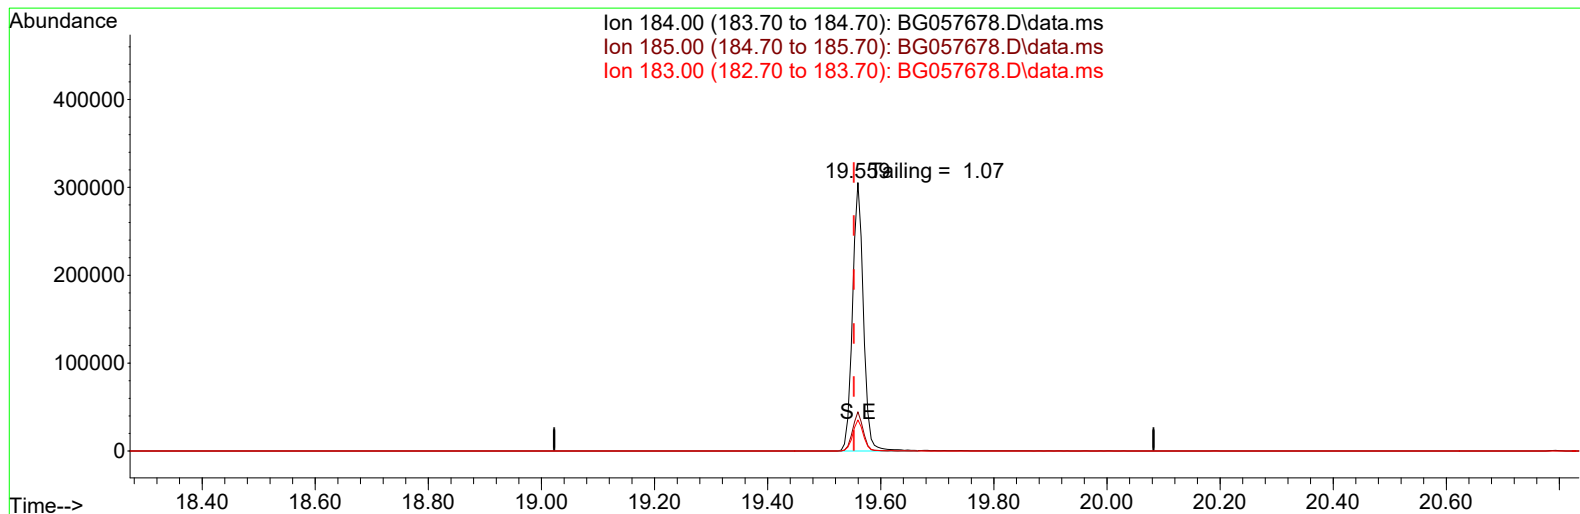

TIC: BG057678.D\data.ms

(77) Benzidine

19.559min (+ 0.007) 0.00 ng

response 408690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.59
183.00	12.10	11.56
0.00	0.00	0.00