
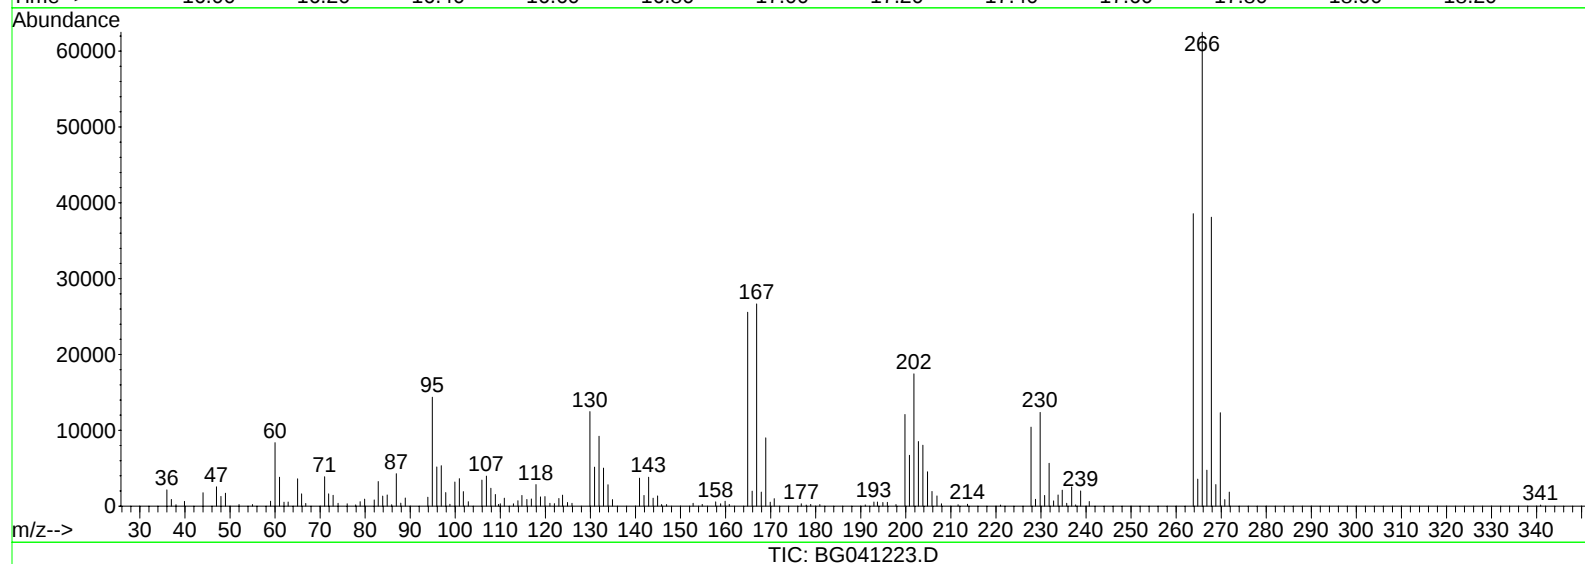


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061319\
Data File : BG041223.D
Acq On : 13 Jun 2019 9:25
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:59:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 23:08:34 2019
Response via : Initial Calibration

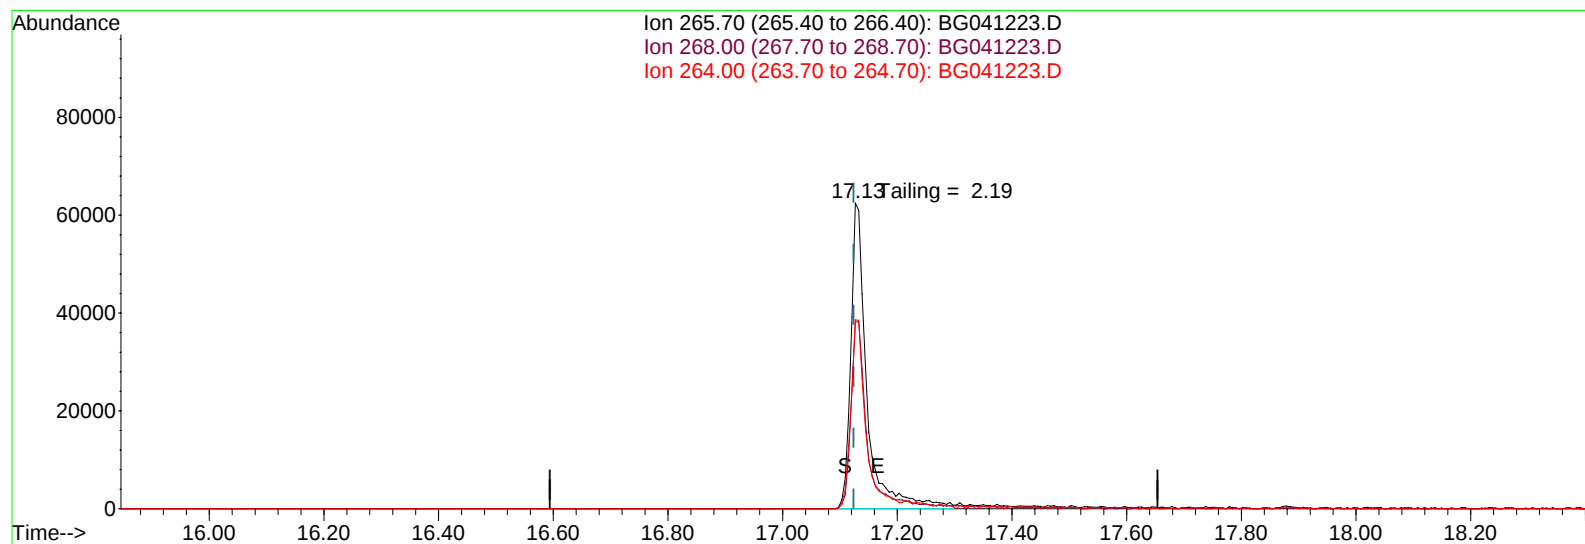

(70) Pentachlorophenol (C)



17.127min (+0.003) 253126.25ng

response 119369

Ion	Exp%	Act%
265.70	100	100
268.00	66.40	60.97
264.00	62.40	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061319\
Data File : BG041223.D
Acq On : 13 Jun 2019 9:25
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:59:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 23:08:34 2019
Response via : Initial Calibration

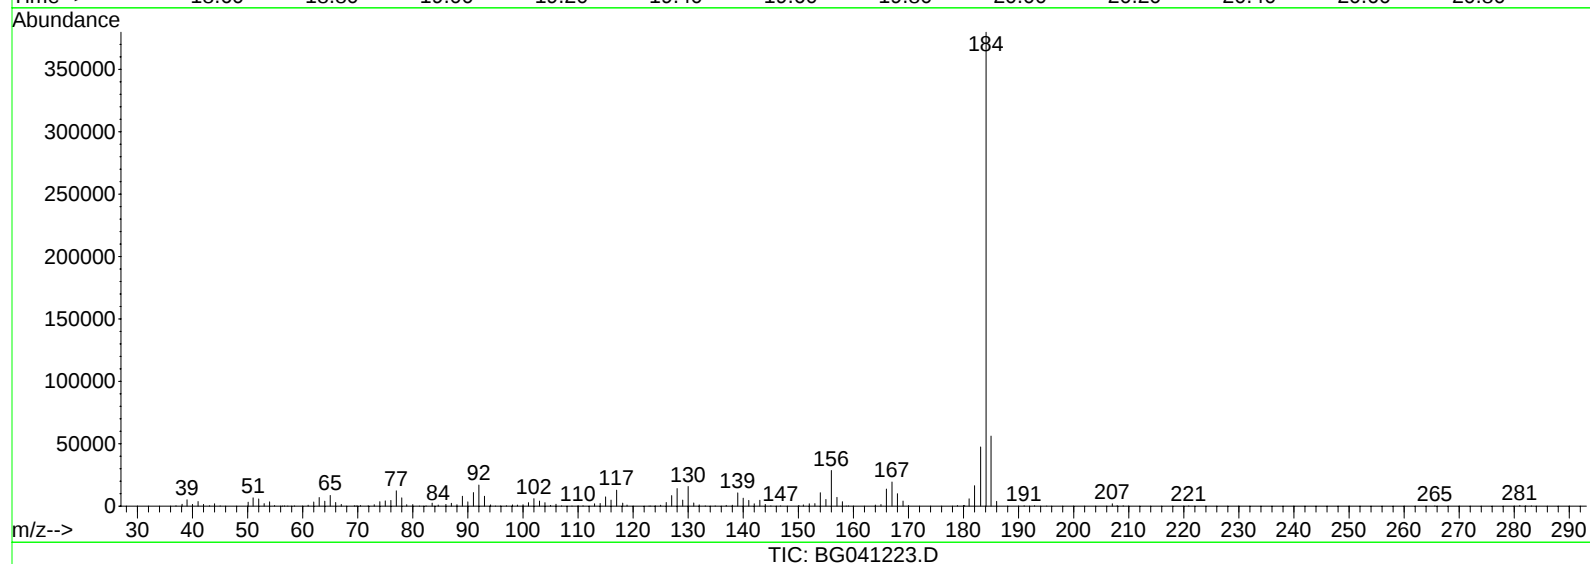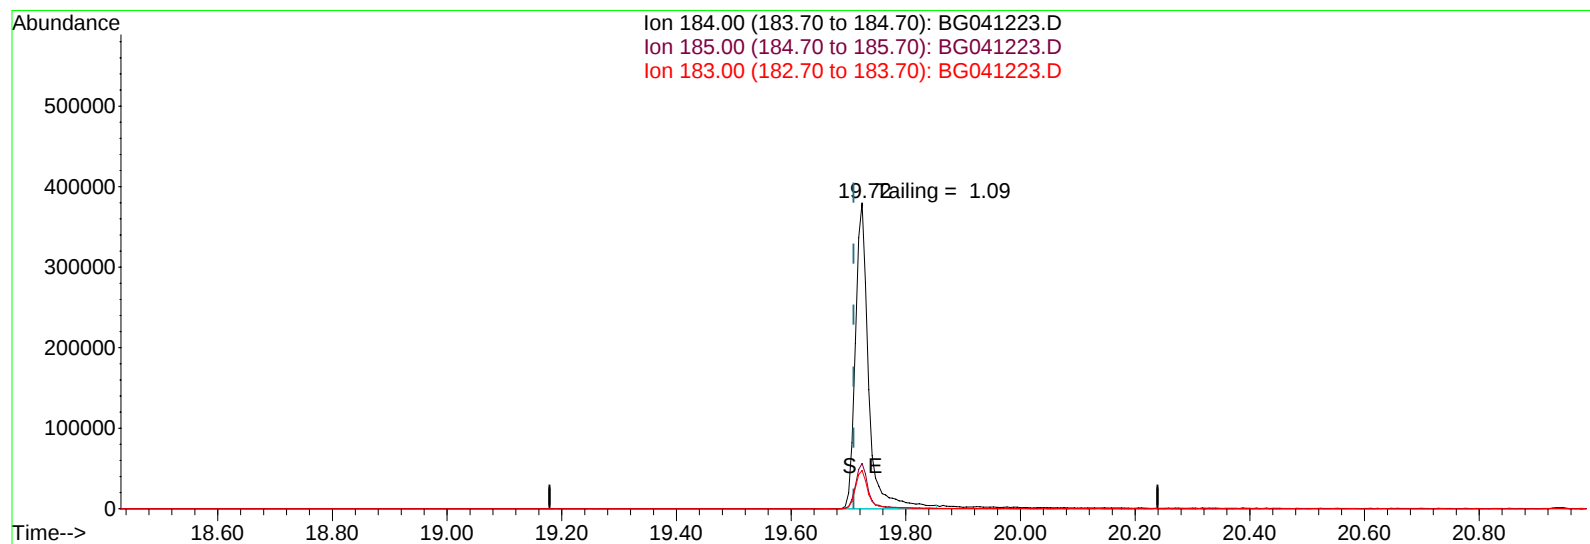

(77) Benzidine

19.724min (+0.015) 352023.99ng

response 613028

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	14.80
183.00	13.40	12.50
0.00	0.00	0.00