
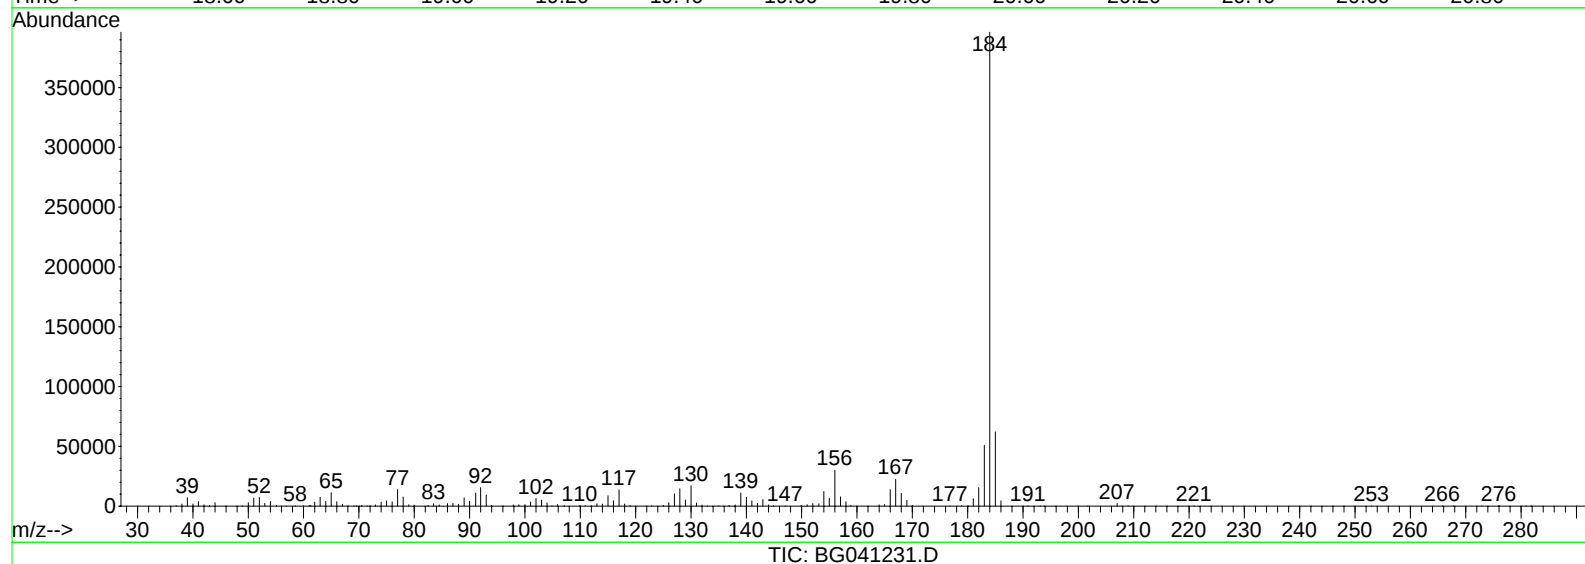


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061319\
Data File : BG041231.D
Acq On : 13 Jun 2019 20:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:08:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 23:08:34 2019
Response via : Initial Calibration

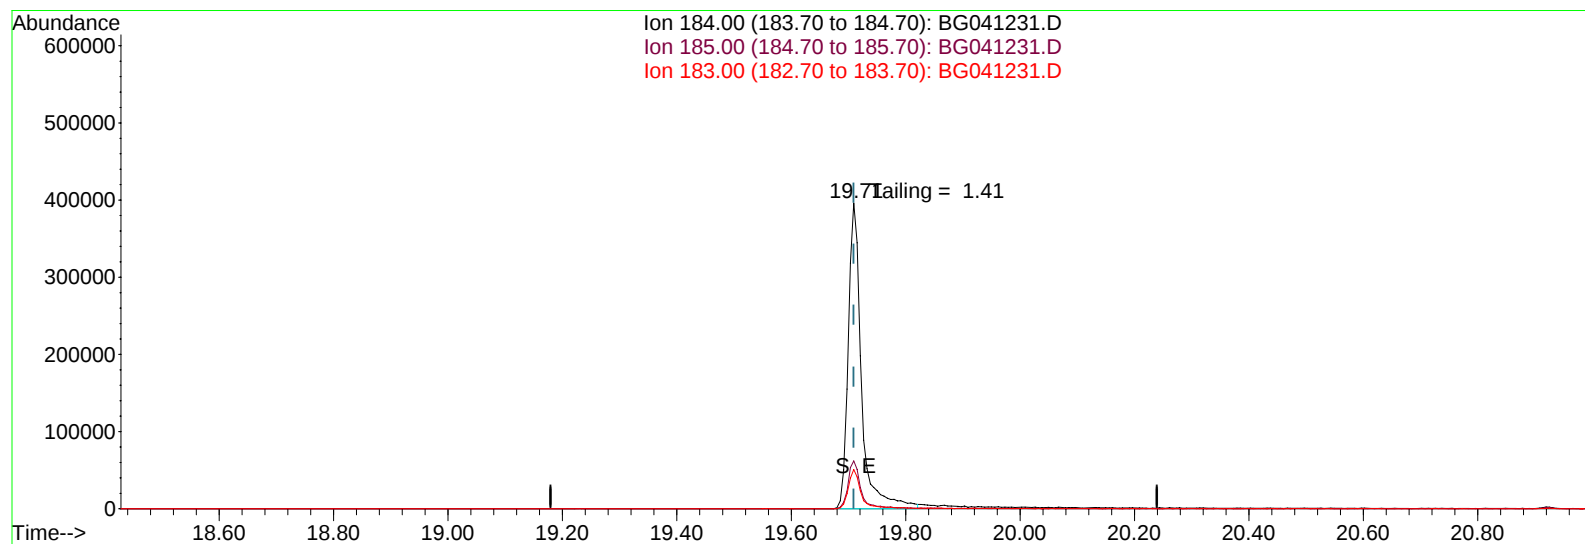

(77) Benzidine



19.709min (0.000) 314855.95ng

response 653456

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.66
183.00	13.40	12.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061319\
Data File : BG041231.D
Acq On : 13 Jun 2019 20:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:08:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG052919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jun 09 23:08:34 2019
Response via : Initial Calibration

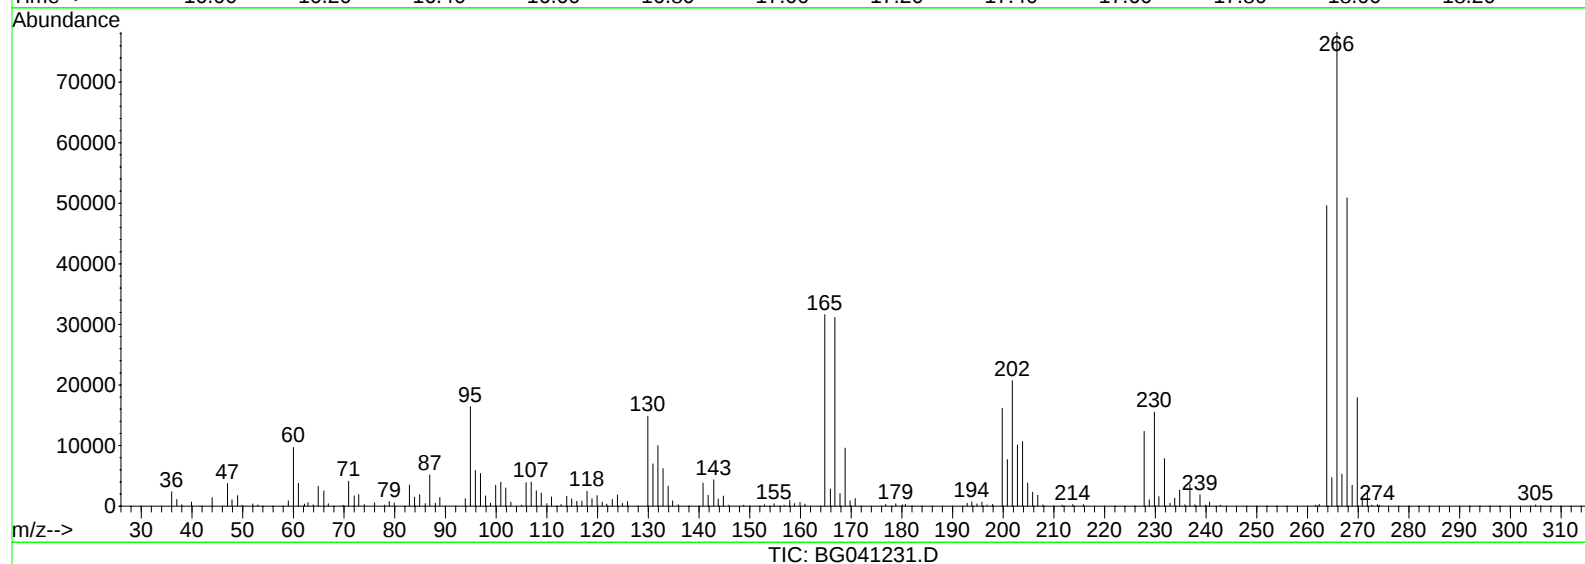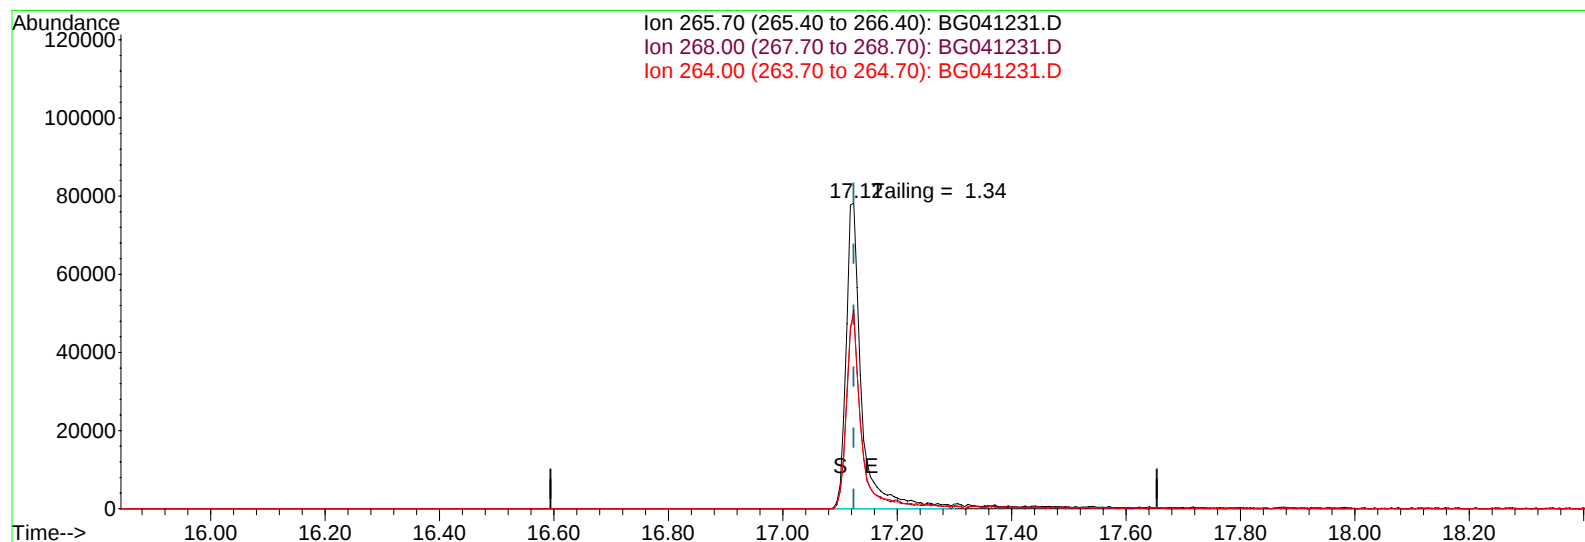

(70) Pentachlorophenol (C)

17.124min (0.000) 292899.57ng

response 145270

Ion	Exp%	Act%
265.70	100	100
268.00	66.40	65.05
264.00	62.40	63.45
0.00	0.00	0.00