


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061319\
 Data File : BG041223.D
 Acq On : 13 Jun 2019 9:25
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG052919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Jun 09 23:08:34 2019

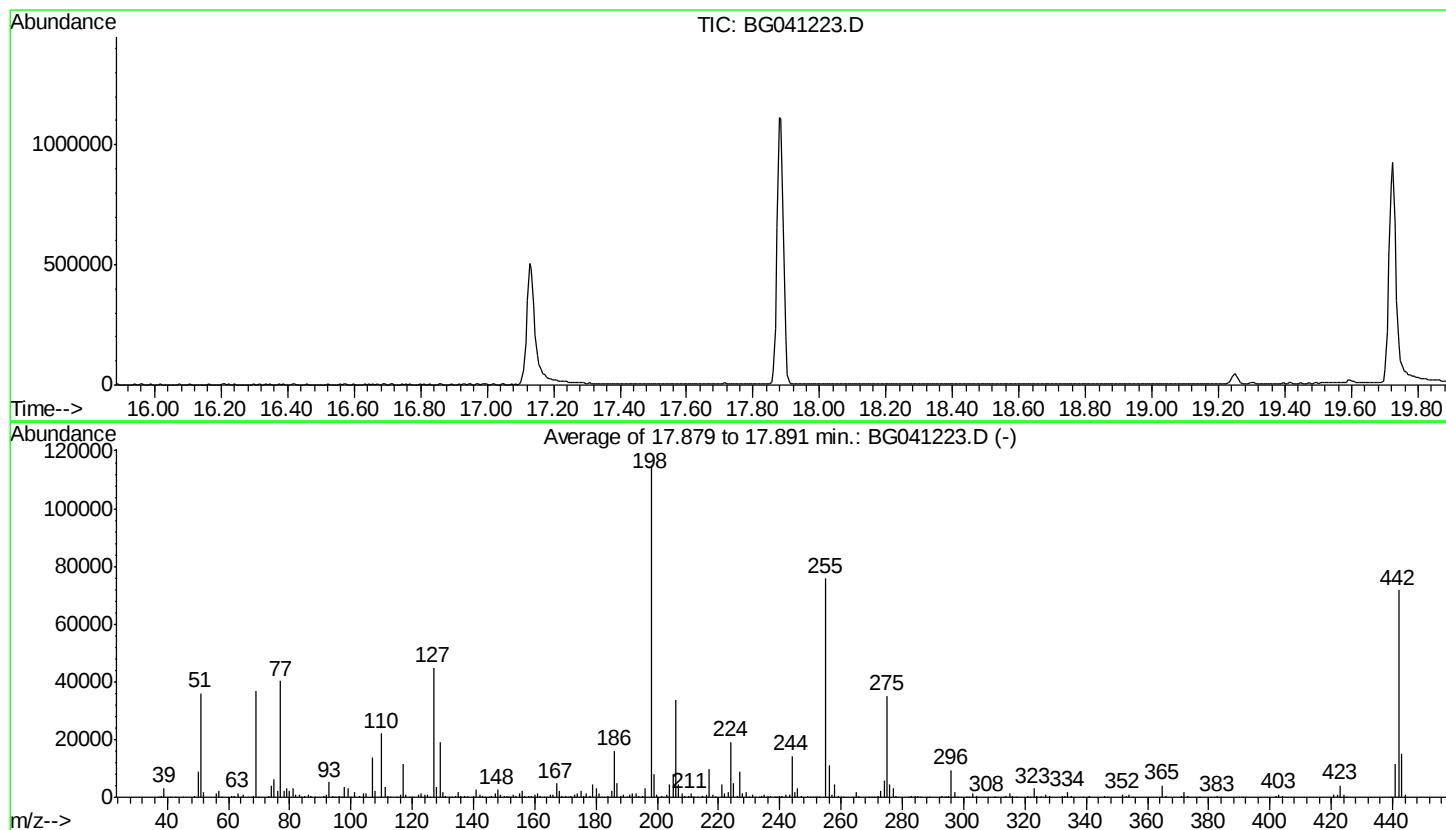

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	36130	PASS
68	69	0.00	2	0.9	327	PASS
69	198	0.00	100	32.0	36808	PASS
70	69	0.00	2	0.4	138	PASS
127	198	10	80	39.0	44813	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114901	PASS
199	198	5	9	6.9	7882	PASS
275	198	10	60	30.5	35080	PASS
365	198	1	100	3.6	4177	PASS
441	198	0.01	100	9.9	11355	PASS
442	198	50	100	62.4	71669	PASS
443	442	15	24	20.9	15008	PASS